

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
 Data File : VV025848.D
 Acq On : 04 May 2022 14:44
 Operator : SY/MD
 Sample : N2670-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	99	rVB	103319	107070	18.29%	2.273%
2	1.571	154	165	179	rBV	103232	118939	20.32%	2.525%
3	2.111	322	333	355	rVB	180336	264456	45.18%	5.614%
4	2.510	447	457	470	rVB	10382	17104	2.92%	0.363%
5	3.899	873	889	929	rBV3	57731	214355	36.62%	4.550%
6	4.352	1014	1030	1061	rBV2	107423	271282	46.35%	5.758%
7	5.050	1231	1247	1273	rBV2	236035	585325	100.00%	12.424%
8	5.619	1412	1424	1450	rBV	162932	333258	56.94%	7.074%
9	5.912	1504	1515	1536	rVB9	3614	7944	1.36%	0.169%
10	6.072	1551	1565	1591	rBV	139081	291693	49.83%	6.192%
11	6.989	1840	1850	1882	rBV	52693	103859	17.74%	2.205%
12	7.317	1941	1952	1982	rBV	260010	460559	78.68%	9.776%
13	7.625	2037	2048	2070	rBV	30763	60308	10.30%	1.280%
14	8.088	2182	2192	2224	rBV	237569	465450	79.52%	9.880%
15	8.419	2285	2295	2307	rBV2	26396	44473	7.60%	0.944%
16	8.850	2418	2429	2449	rBV	267984	445126	76.05%	9.449%
17	10.217	2841	2854	2868	rBV	86830	138986	23.75%	2.950%
18	11.246	3163	3174	3190	rBV	258676	404512	69.11%	8.586%
19	11.622	3280	3291	3311	rBV	238100	376358	64.30%	7.989%




Sum of corrected areas: 4711057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025848.D
Acq On : 04 May 2022 14:44
Operator : SY/MD
Sample : N2670-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

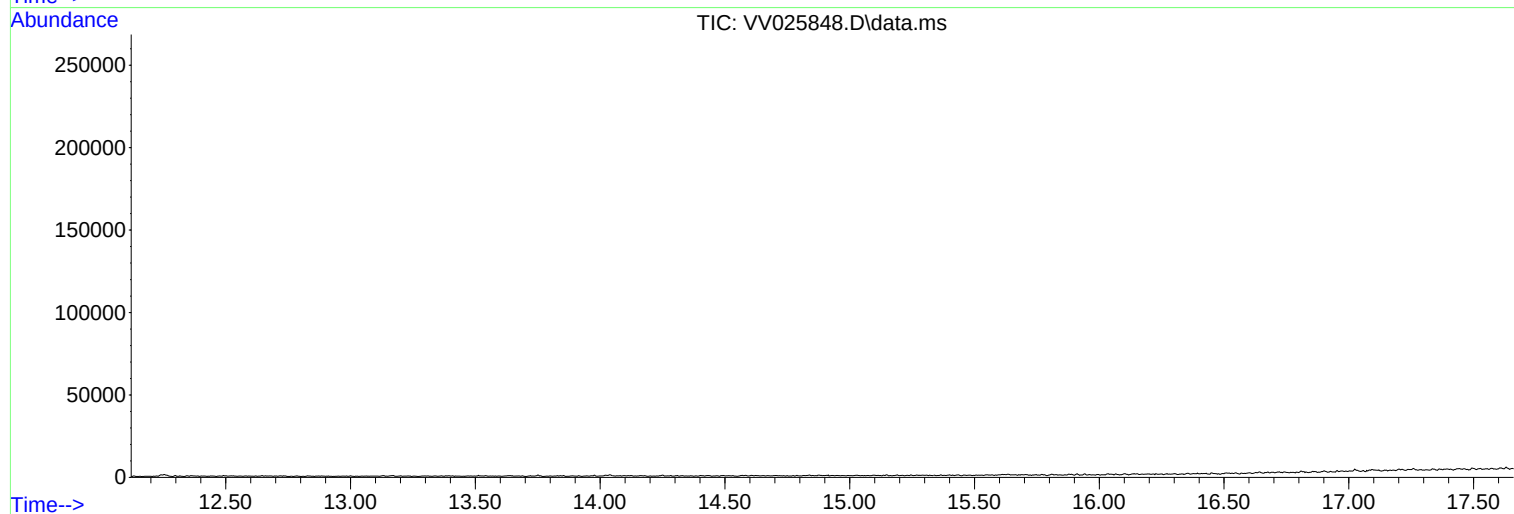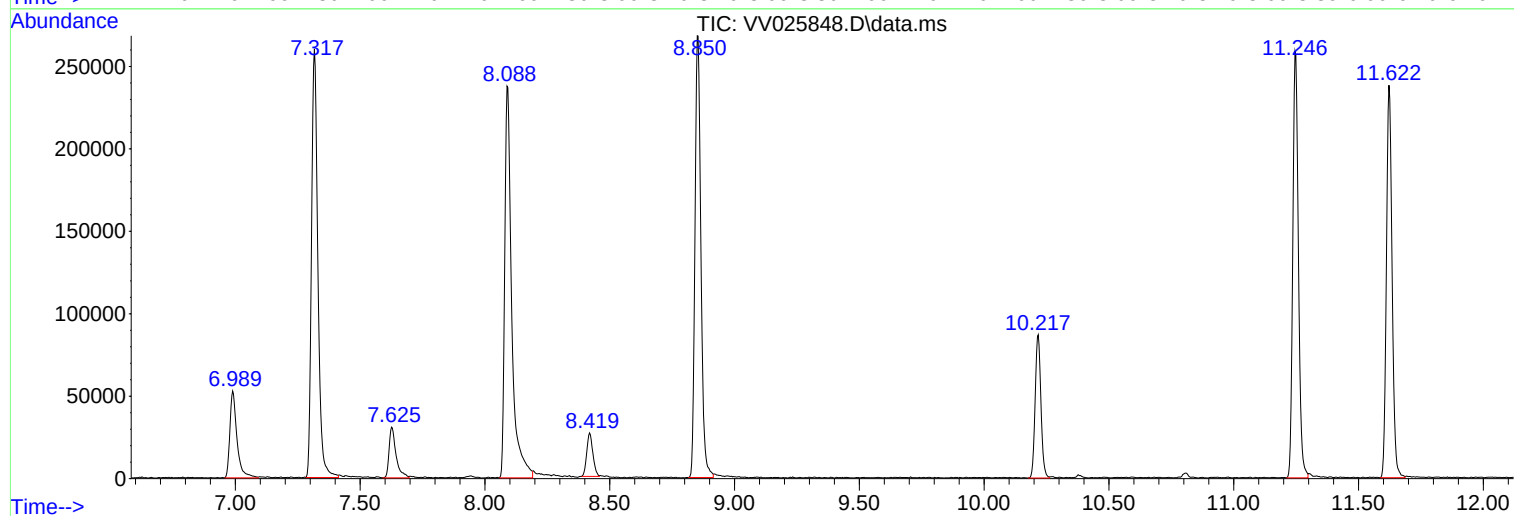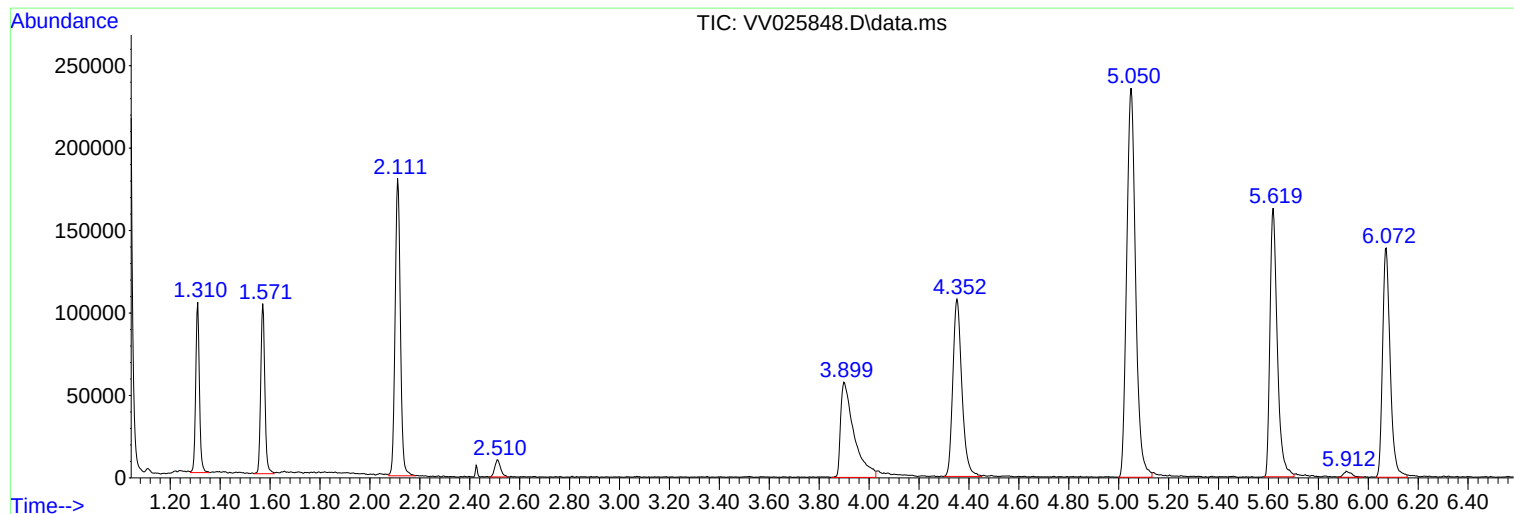

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025848.D
Acq On : 04 May 2022 14:44
Operator : SY/MD
Sample : N2670-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
Data File : VV025848.D
Acq On : 04 May 2022 14:44
Operator : SY/MD
Sample : N2670-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc