
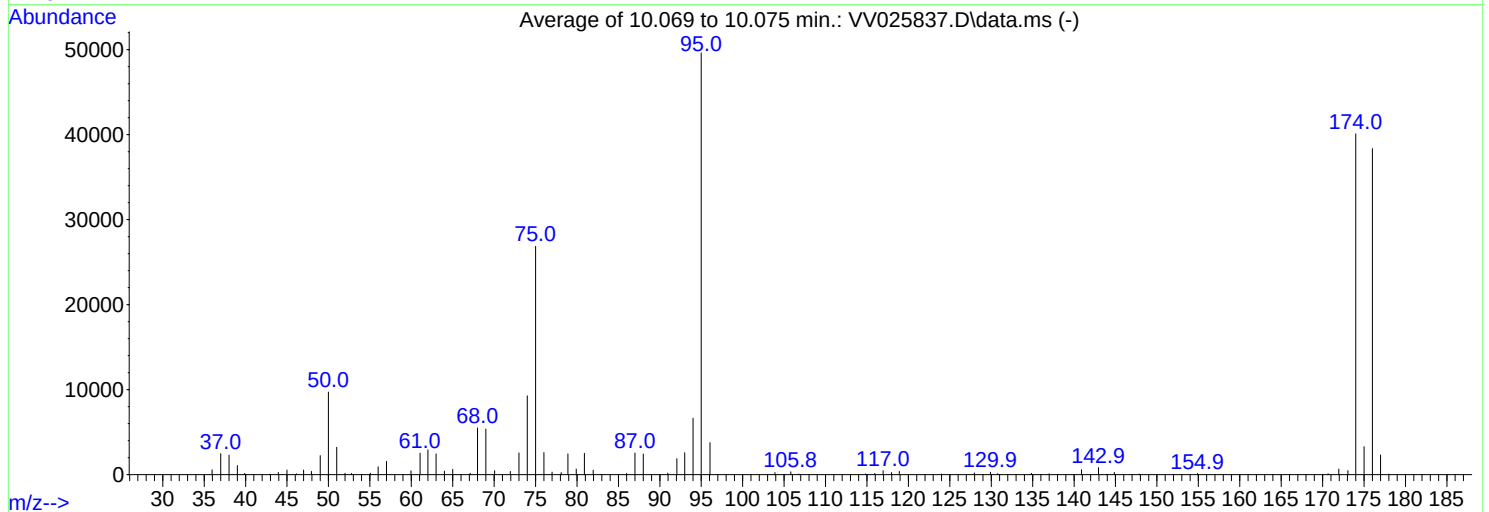


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050422\
 Data File : VV025837.D
 Acq On : 04 May 2022 09:40
 Operator : SY/MD
 Sample : BFB314
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB314

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR050322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu May 05 04:55:53 2022

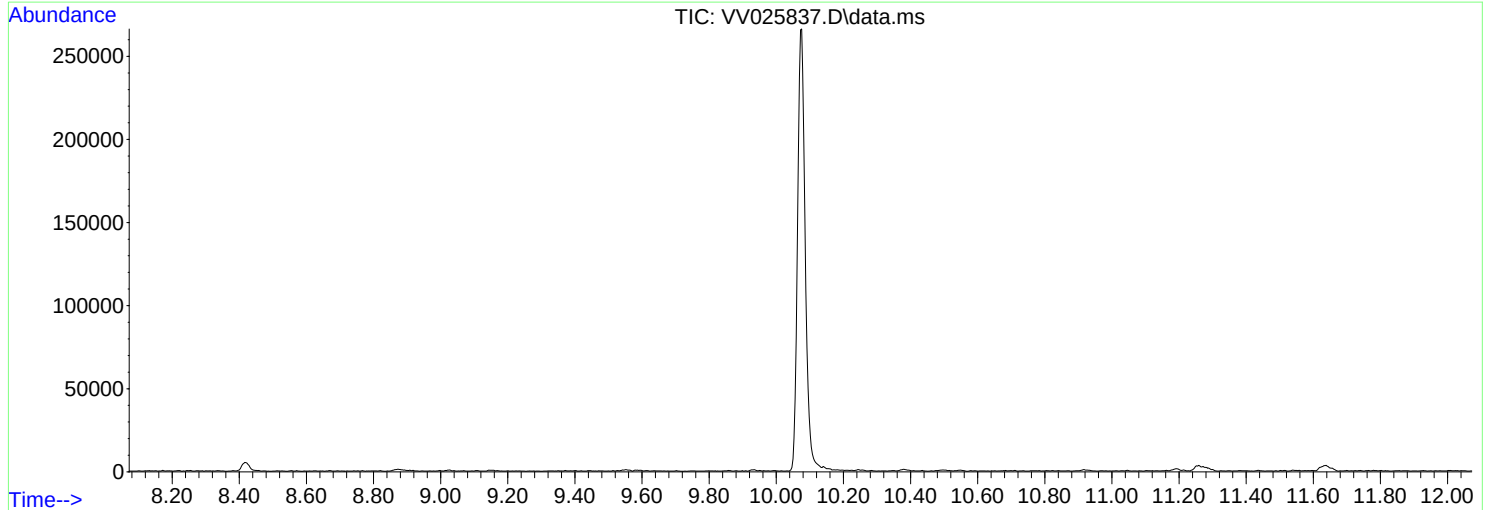

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	9709	PASS
75	95	30	80	54.1	26872	PASS
95	95	100	100	100.0	49629	PASS
96	95	5	9	7.6	3771	PASS
173	174	0.00	2	1.2	475	PASS
174	95	50	120	80.8	40104	PASS
175	174	5	9	8.2	3294	PASS
176	174	95	105	95.7	38360	PASS
177	176	5	10	6.1	2325	PASS

m/z	Abundance
39.90	156.0
43.90	401.0

Instrument :
MSVOA_V
ClientSampleId :
BFB314

m/z	Abundance
36.00	491.0
37.00	2319.0
38.00	2141.0
39.00	1079.0
39.90	257.0
42.90	114.0
44.00	715.0
45.00	462.0
47.00	523.0
47.90	356.0
49.00	2151.0
50.00	8977.0
51.00	3081.0
52.00	154.0
52.80	152.0
55.00	175.0
56.00	860.0
57.00	1467.0
59.90	463.0
61.00	2427.0
62.00	2687.0
63.00	2445.0
64.00	441.0
65.00	521.0
67.20	143.0
68.00	5240.0
69.00	4880.0
70.10	454.0
72.00	318.0
73.00	2416.0
74.00	8691.0
75.00	25248.0
76.00	2420.0
76.90	306.0
78.10	183.0
78.90	2303.0
79.90	662.0
80.90	2354.0
81.90	475.0
82.80	100.0
86.00	135.0
87.00	2378.0
88.00	2187.0
91.00	186.0
92.00	1736.0
93.00	2430.0
94.00	6009.0
95.00	46584.0
96.10	3497.0
103.90	207.0
105.10	103.0
105.80	348.0
106.80	112.0
115.90	138.0
117.00	449.0
118.00	247.0
118.90	407.0
128.00	194.0
129.90	306.0
130.80	156.0
134.80	151.0
137.00	113.0
140.90	532.0
143.00	653.0
144.90	230.0
154.90	123.0
170.70	136.0
171.90	603.0
173.10	477.0
174.00	36472.0
175.00	3136.0
176.00	34528.0
177.00	2121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB314

m/z	Abundance
35.90	588.0
37.00	2558.0
38.00	2316.0
39.00	1112.0
39.90	303.0
44.00	691.0
45.00	562.0
46.20	118.0
47.00	570.0
47.90	394.0
49.00	2314.0
50.00	9938.0
51.00	3317.0
52.00	158.0
52.80	163.0
55.10	166.0
56.00	952.0
57.00	1598.0
59.90	462.0
61.00	2585.0
62.00	2978.0
63.00	2558.0
64.00	444.0
65.00	652.0
67.10	170.0
68.00	5729.0
69.00	5577.0
70.00	473.0
71.90	400.0
73.00	2657.0
74.00	9632.0
75.00	27928.0
76.00	2746.0
77.00	300.0
78.10	255.0
78.90	2546.0
79.90	677.0
80.90	2617.0
81.90	555.0
86.00	137.0
87.00	2634.0
88.00	2554.0
91.00	193.0
92.00	1975.0
93.00	2699.0
94.00	6959.0
95.00	51480.0
96.00	4005.0
103.90	247.0
105.80	386.0
106.80	109.0
114.90	124.0
116.00	163.0
117.00	481.0
117.90	252.0
118.90	412.0
124.00	108.0
128.00	192.0
129.90	296.0
130.80	135.0
134.80	153.0
137.00	120.0
140.90	621.0
143.00	829.0
144.80	277.0
147.90	120.0
154.90	140.0
170.70	116.0
171.90	690.0
173.10	468.0
174.00	41496.0
175.00	3433.0
176.00	39728.0
177.00	2391.0
178.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB314

m/z	Abundance
35.90	591.0
37.00	2524.0
38.00	2429.0
39.00	1030.0
39.90	384.0
44.00	605.0
45.00	607.0
46.10	140.0
47.00	560.0
48.00	379.0
49.00	2277.0
50.00	10211.0
51.00	3247.0
52.00	175.0
52.80	144.0
55.00	164.0
56.00	937.0
57.00	1653.0
60.00	435.0
61.10	2567.0
62.00	3072.0
63.00	2339.0
64.00	388.0
65.00	689.0
67.00	212.0
68.00	5520.0
69.00	5640.0
70.00	505.0
71.90	409.0
73.00	2628.0
74.00	9503.0
75.00	27440.0
76.00	2651.0
77.10	317.0
78.10	278.0
78.90	2502.0
79.90	629.0
80.90	2552.0
82.00	571.0
83.00	102.0
86.00	156.0
87.00	2629.0
88.00	2522.0
90.90	198.0
92.10	1949.0
93.00	2599.0
94.00	6973.0
95.00	50824.0
96.00	3811.0
103.90	278.0
105.80	312.0
114.80	133.0
115.90	172.0
116.90	485.0
117.90	235.0
118.90	370.0
124.00	125.0
127.90	213.0
129.90	263.0
130.80	116.0
134.90	139.0
137.00	114.0
140.90	603.0
142.90	992.0
143.90	111.0
144.80	290.0
145.90	103.0
147.80	108.0
154.90	141.0
157.00	110.0
170.60	109.0
172.00	714.0
172.90	480.0
174.00	42344.0
175.00	3314.0
176.00	40824.0
177.00	2463.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB314