

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050423\
 Data File : VV030986.D
 Acq On : 04 May 2023 12:22
 Operator : SY/MD
 Sample : VV0504WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

Quant Time: May 05 05:14:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM050223.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 03 06:25:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	4013	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.800	117	3757	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2105	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	1652	0.485	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	96.000%
4) 1,2-Dichloroethane-d4	4.969	65	1569	0.541	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	5.995	67	1442	0.579	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	116.000%
8) Toluene-d8	7.253	98	5060	0.556	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	112.000%
10) 1,1,2,2-Tetrachloroeth...	10.163	84	1138	0.583	ug/L	0.02
Spiked Amount	0.500	Range	65 - 120	Recovery	=	116.000%
Target Compounds						
6) Trichloroethene	5.852	95	64	0.022	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050423\
Data File : VV030986.D
Acq On : 04 May 2023 12:22
Operator : SY/MD
Sample : VV0504WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211


Quant Time: May 05 05:14:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM050223.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 03 06:25:35 2023
Response via : Initial Calibration

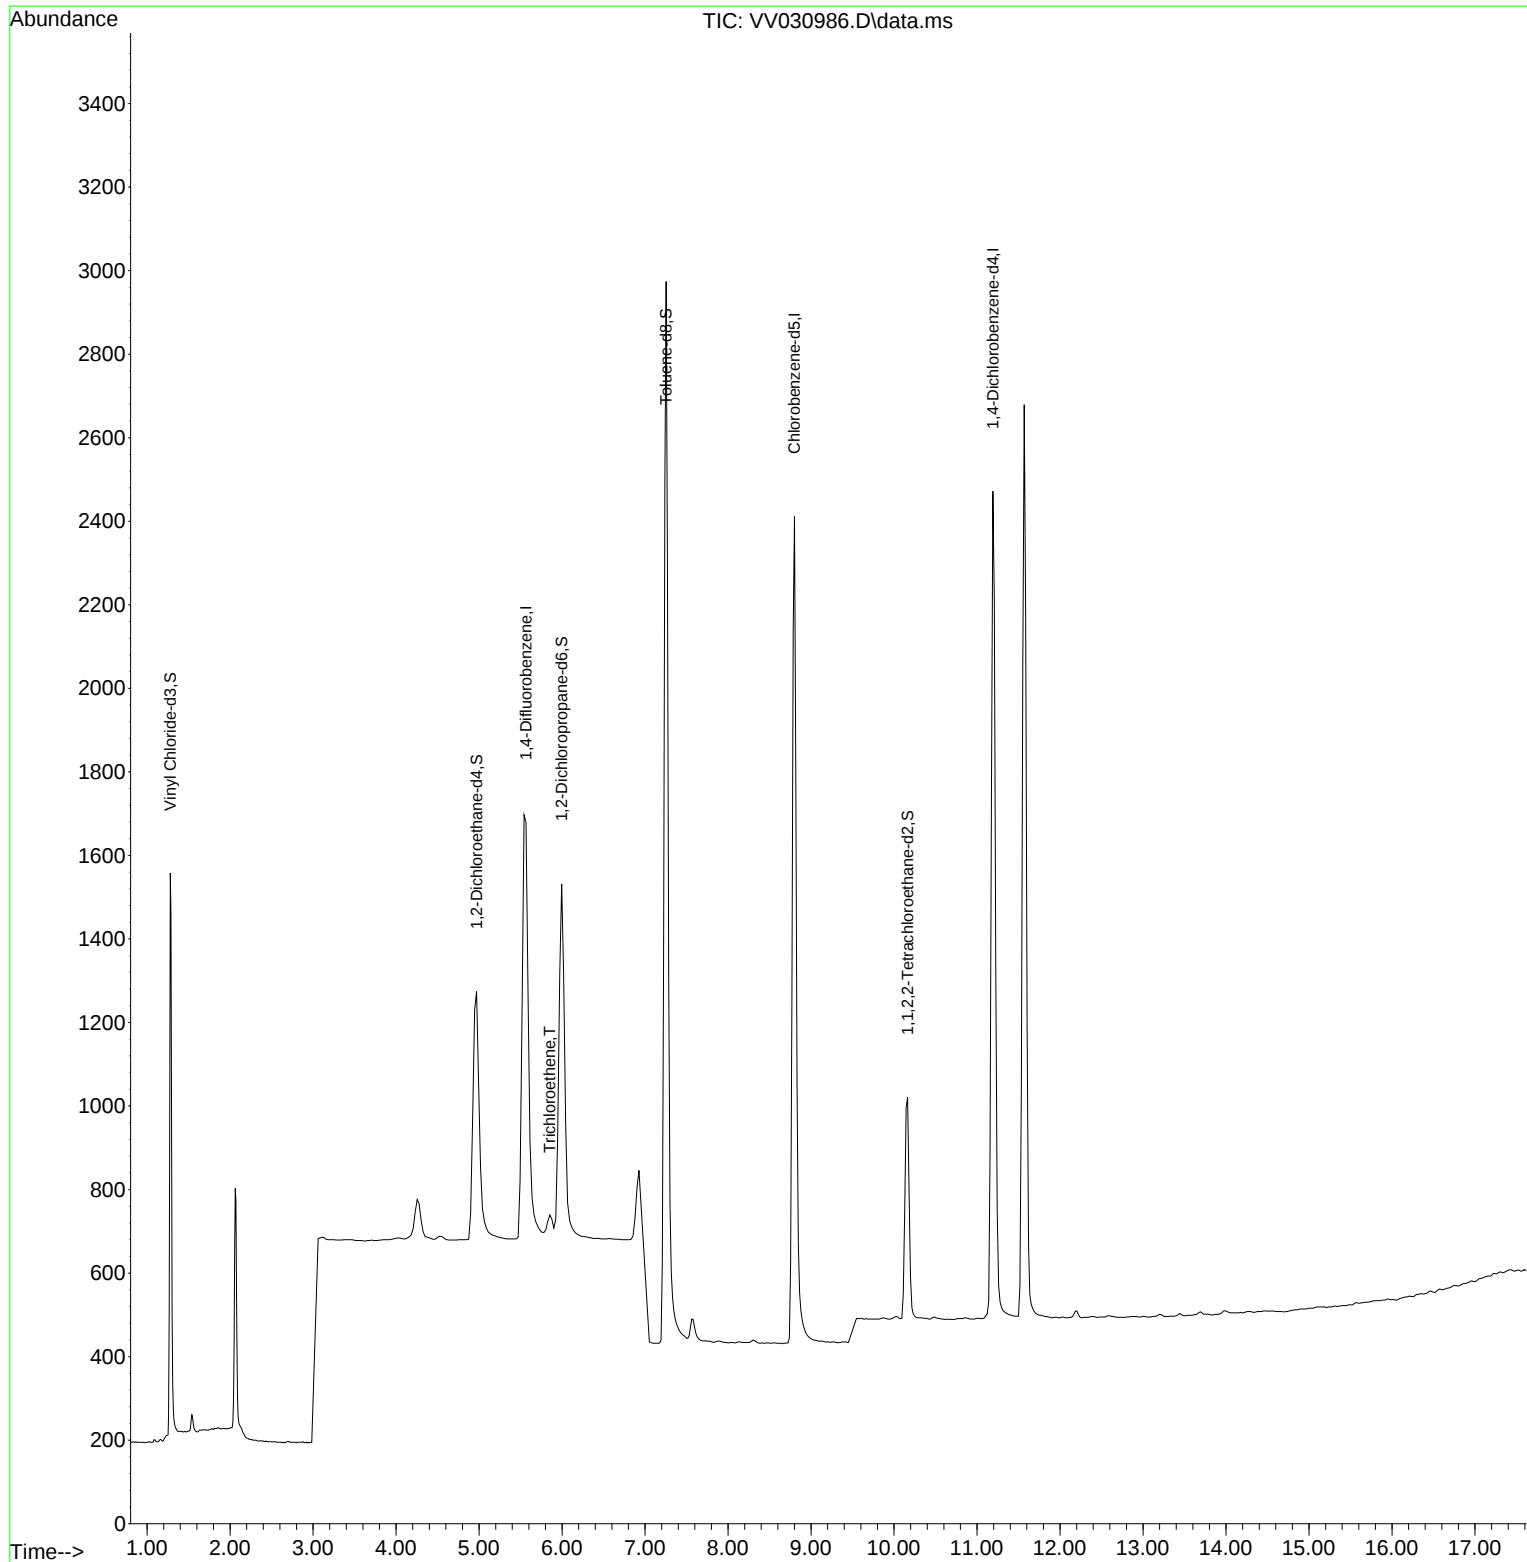

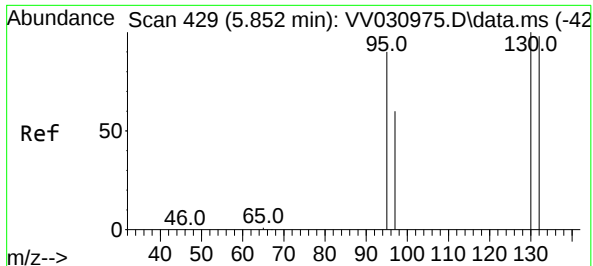

#6
 Trichloroethene
 Concen: 0.022 ug/L
 RT: 5.852 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VV030986.D
 Acq: 04 May 2023 12:22

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

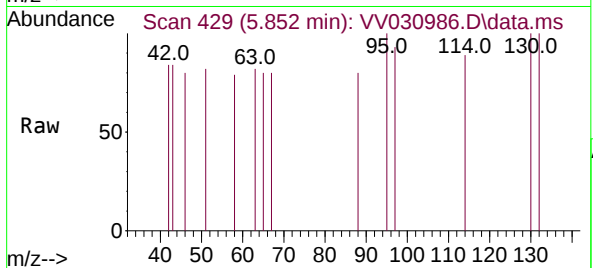

Tgt Ion: 95	Resp: 64
Ion Ratio	Lower Upper
95 100	
97 93.4	49.6 92.2#
132 100.0	76.2 141.4
130 100.0	77.2 143.4

