
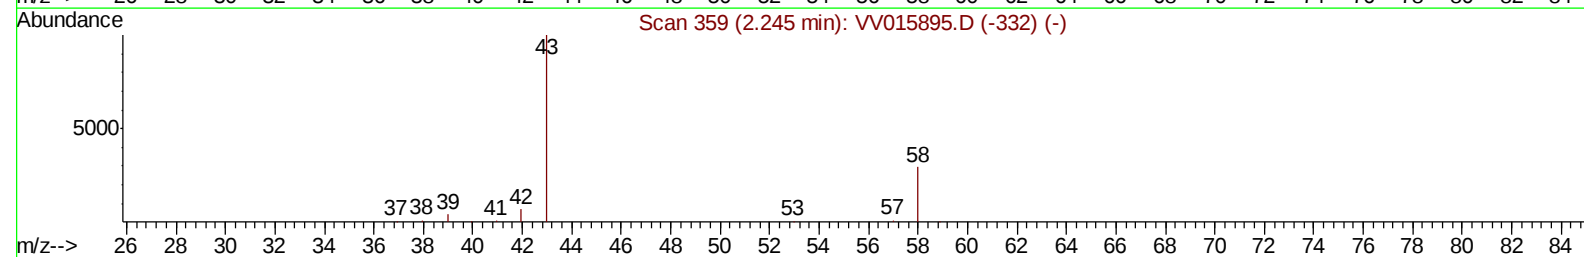
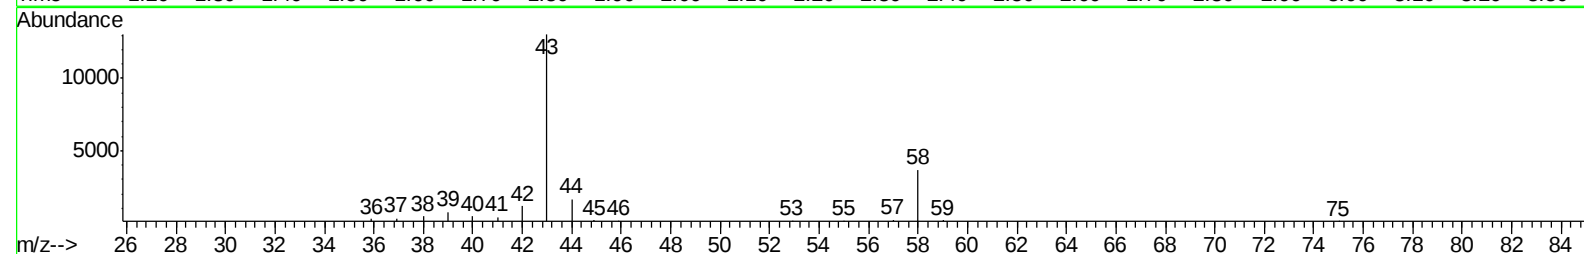


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050520\
Data File : VV015898.D
Acq On : 05 May 2020 13:11
Operator : SY/MD
Sample : VSTDICV005
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 06 01:58:44 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050520WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 05 17:59:17 2020
Response via : Initial Calibration

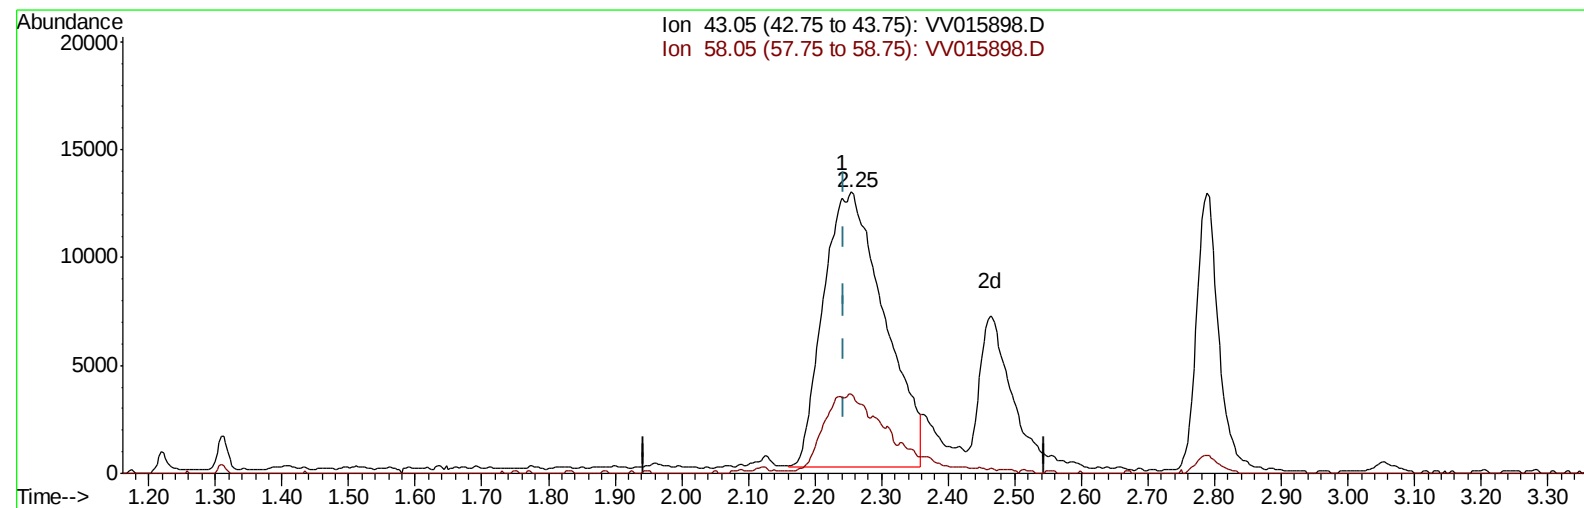

TIC: VV015898.D

(13) Acetone (T)

2.254min (+0.010) 50.20ug/L m

response 80547

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	10.12
0.00	0.00	0.00
0.00	0.00	0.00