


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV050520\
 Data File : VV015892.D
 Acq On : 05 May 2020 09:15
 Operator : SY/MD
 Sample : BFB50
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB50

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050520WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue May 05 17:59:17 2020

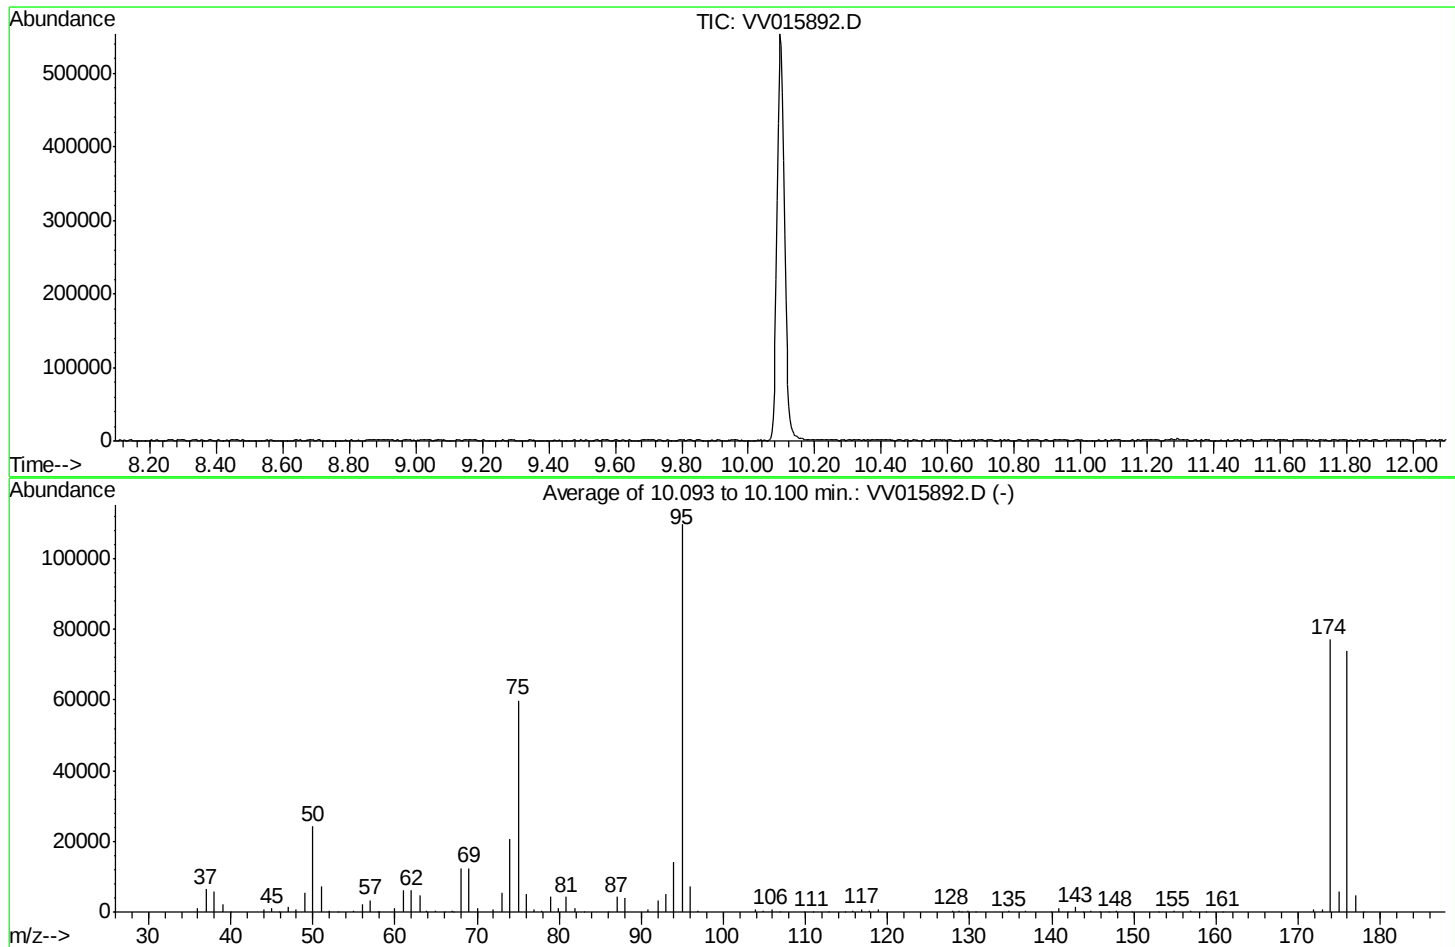

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	24266	PASS
75	95	30	80	54.5	59856	PASS
95	95	100	100	100.0	109736	PASS
96	95	5	9	6.5	7171	PASS
173	174	0.00	2	1.0	764	PASS
174	95	50	120	70.2	77024	PASS
175	174	5	9	7.6	5832	PASS
176	174	95	101	95.9	73829	PASS
177	176	5	9	6.6	4894	PASS

m/z	Abundance
36.00	1113.0
37.00	6282.0
38.00	5845.0
39.00	2156.0
40.00	488.0
44.00	1039.0
45.00	1086.0
45.90	116.0
47.00	1474.0
47.90	693.0
49.00	5311.0
50.00	23920.0
51.00	7375.0
52.00	366.0
55.00	407.0
56.00	2026.0
57.00	3196.0
57.90	125.0
58.10	121.0
60.00	1145.0
61.00	5979.0
62.00	6080.0
63.00	4743.0
63.90	510.0
65.00	509.0
66.00	139.0
66.90	353.0
68.00	11688.0
69.00	12053.0
70.00	937.0
71.90	597.0
73.00	5541.0
74.00	20080.0
75.00	58432.0
76.00	4974.0
77.00	750.0
77.80	347.0
78.90	4197.0
79.90	1175.0
80.90	4309.0
81.90	951.0
85.90	212.0
87.00	4008.0
88.00	3679.0
90.90	551.0
92.00	3339.0
93.00	4987.0
94.00	13432.0
95.00	105768.0
96.00	6999.0
97.00	197.0
103.90	506.0
104.90	232.0
105.90	629.0
106.80	103.0
109.80	131.0
110.90	110.0
112.90	140.0
115.80	405.0
116.90	773.0
117.80	437.0
118.80	610.0
127.90	345.0
128.80	248.0
129.80	341.0
130.80	202.0
134.80	221.0
136.80	224.0
140.80	1161.0
141.90	106.0
142.90	1266.0
143.80	114.0
144.80	186.0
145.90	151.0
147.90	204.0
149.80	143.0
154.90	348.0
156.90	202.0
158.90	120.0
160.90	149.0
171.90	576.0
173.90	72624.0
175.00	5529.0
175.90	69248.0
177.00	4644.0
178.00	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	1178.0
37.00	6570.0
38.00	6005.0
39.00	2192.0
40.00	541.0
44.00	1087.0
45.00	1137.0
45.90	142.0
47.00	1553.0
47.90	706.0
49.00	5456.0
50.00	25176.0
51.00	7470.0
52.00	388.0
53.00	101.0
54.90	406.0
56.00	2118.0
57.00	3409.0
57.90	153.0
60.00	1193.0
61.00	6281.0
62.00	6306.0
63.00	5026.0
63.90	507.0
65.00	467.0
66.00	145.0
66.90	311.0
68.00	12559.0
69.00	12789.0
70.00	1017.0
71.90	684.0
73.00	5652.0
74.00	21408.0
75.00	61888.0
76.00	5174.0
76.90	807.0
77.80	348.0
78.90	4480.0
79.90	1258.0
80.90	4446.0
81.90	1075.0
83.00	111.0
85.90	187.0
87.00	4326.0
88.00	4254.0
90.90	586.0
92.00	3429.0
93.00	5384.0
94.00	14549.0
95.00	113632.0
96.00	7459.0
96.90	242.0
103.80	573.0
104.90	262.0
105.90	649.0
106.80	112.0
109.80	116.0
110.90	109.0
112.70	142.0
113.00	135.0
114.80	137.0
115.80	443.0
116.90	819.0
117.80	481.0
118.80	686.0
127.90	395.0
128.80	240.0
129.80	333.0
130.80	196.0
134.80	266.0
136.80	230.0
140.00	109.0
140.80	1247.0
142.90	1369.0
143.90	120.0
144.80	214.0
145.90	165.0
147.00	104.0
147.90	253.0
149.80	160.0
153.00	102.0
154.90	349.0
156.90	256.0
158.80	172.0
160.90	173.0
171.90	584.0
173.00	1142.0
173.90	79240.0
175.00	6014.0
175.90	76280.0
177.00	5079.0
178.00	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	1155.0
37.00	6310.0
38.00	5511.0
39.00	2146.0
40.00	554.0
44.00	1079.0
45.00	1040.0
46.00	156.0
47.00	1444.0
47.90	688.0
49.00	5113.0
50.00	23704.0
51.00	7035.0
52.00	362.0
53.00	138.0
54.90	389.0
56.00	1935.0
57.00	3385.0
57.90	179.0
60.00	1186.0
61.00	5889.0
62.00	5861.0
63.00	4764.0
63.90	448.0
65.00	429.0
66.00	109.0
67.10	288.0
68.00	12240.0
69.00	12386.0
70.00	994.0
71.90	626.0
73.00	5264.0
74.00	20816.0
75.00	59248.0
76.00	4886.0
76.90	728.0
77.90	329.0
78.90	4245.0
79.90	1206.0
80.90	4245.0
81.90	1017.0
82.90	125.0
86.00	171.0
87.00	4267.0
87.90	4318.0
90.80	549.0
92.00	3328.0
93.00	5219.0
94.00	14119.0
95.00	109808.0
96.00	7057.0
96.90	249.0
103.80	647.0
104.90	245.0
105.90	631.0
106.80	125.0
110.80	121.0
112.70	134.0
114.80	159.0
115.80	432.0
116.90	772.0
117.80	486.0
118.80	681.0
127.90	424.0
128.70	182.0
129.00	188.0
129.80	327.0
130.80	170.0
134.80	270.0
136.80	223.0
139.90	124.0
140.80	1231.0
142.90	1346.0
144.80	218.0
145.90	165.0
147.00	122.0
147.80	273.0
149.80	151.0
153.10	106.0
154.80	307.0
156.90	244.0
158.70	198.0
160.80	153.0
171.90	572.0
173.00	1151.0
173.90	79208.0
175.00	5955.0
175.90	75960.0
177.00	4959.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

Scan 2788 (10.055 min): VV015892.D
BFB50

m/z	Abundance
35.90	105.0
39.90	408.0
44.00	380.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50