

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021281.D
 Acq On : 05 May 2021 10:05
 Operator : SY/MD
 Sample : VV0505MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 06 02:16:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 06 02:15:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	691159	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	654798	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	332037	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	119787	39.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.14%
7) Chloroethane-d5	1.571	69	119554	43.64	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.28%
11) 1,1-Dichloroethene-d2	2.108	63	249132	29.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.26%#
21) 2-Butanone-d5	3.899	46	220216	89.51	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.51%
24) Chloroform-d	4.349	84	444604	45.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.12%
26) 1,2-Dichloroethane-d4	5.034	65	343993	47.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.18%
32) Benzene-d6	5.050	84	717831	47.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.20%
36) 1,2-Dichloropropane-d6	6.072	67	188203	48.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.18%
41) Toluene-d8	7.317	98	718576	45.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.96%
43) trans-1,3-Dichloroprop...	7.625	79	131220	45.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.08%
47) 2-Hexanone-d5	8.091	63	153725	85.94	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.94%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	286260	46.18	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.36%
66) 1,2-Dichlorobenzene-d4	11.632	152	331930	50.73	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.46%
Target Compounds						
39) cis-1,3-Dichloropropene	6.992	75	9252	1.34	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021281.D
Acq On : 05 May 2021 10:05
Operator : SY/MD
Sample : VV0505MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: May 06 02:16:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 06 02:15:40 2021
Response via : Initial Calibration

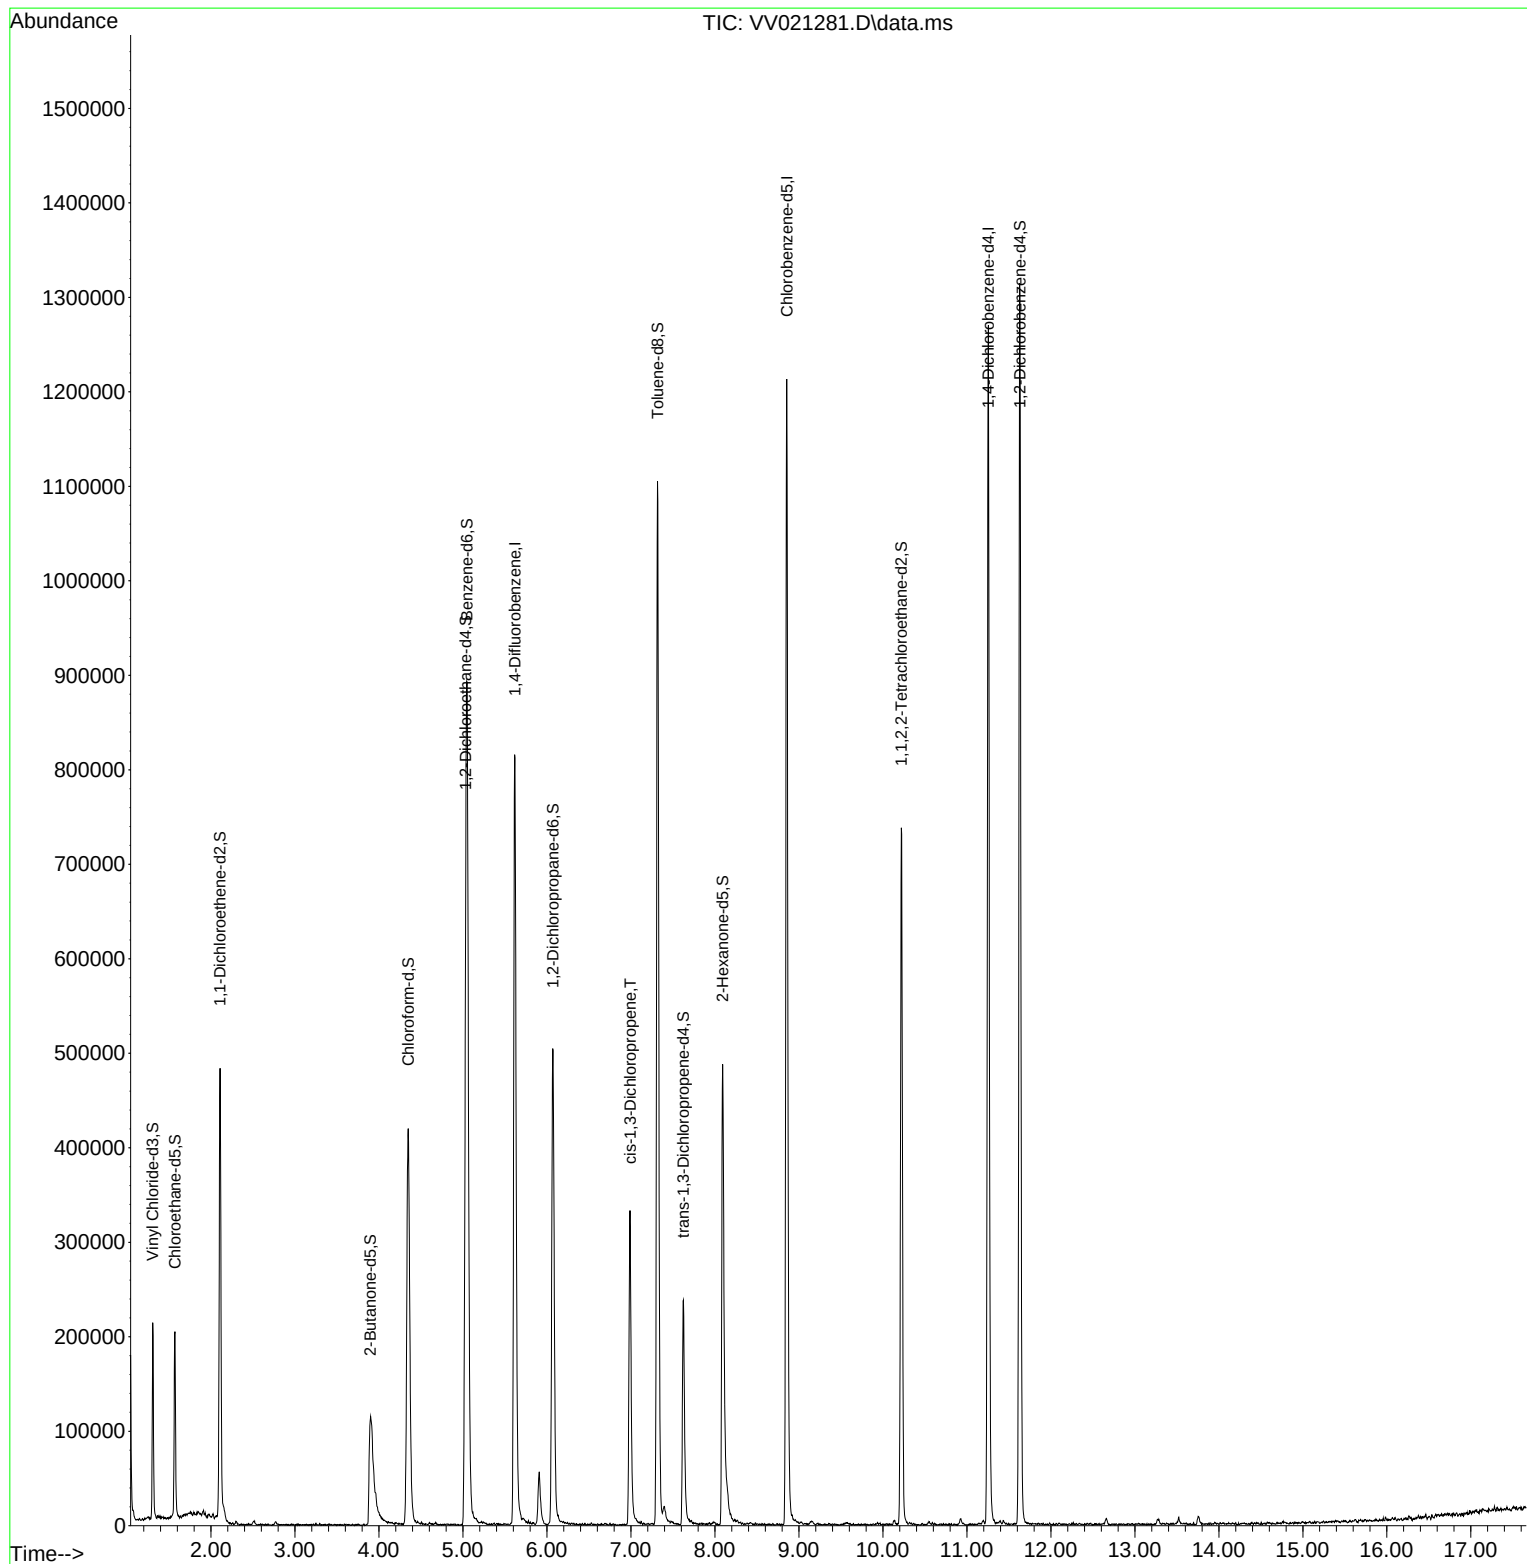

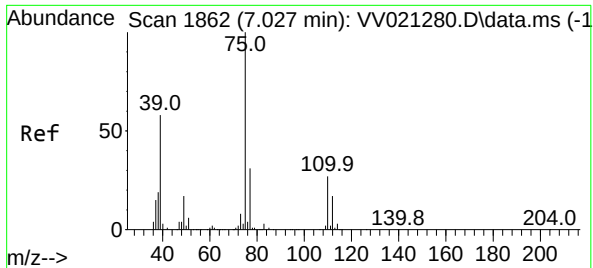

#39
 cis-1,3-Dichloropropene
 Concen: 1.34 ug/L
 RT: 6.992 min Scan# 1851
 Delta R.T. -0.035 min
 Lab File: VV021281.D
 Acq: 05 May 2021 10:05

Instrument :
 MSVOA_V
 ClientSampleId :

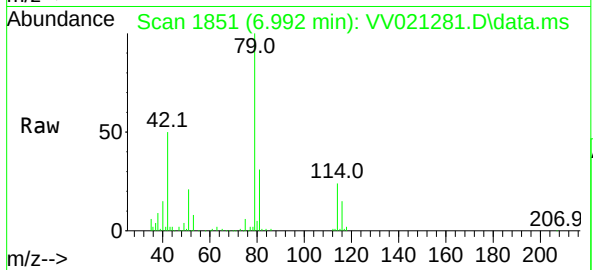

Tgt Ion: 75 Resp: 9252
 Ion Ratio Lower Upper
 75 100
 77 38.1 21.8 40.6

