

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021290.D
 Acq On : 05 May 2021 14:07
 Operator : SY/MD
 Sample : M2249-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 06 02:18:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 06 02:15:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	691394	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	655012	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	334562	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	179035	58.38	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	116.76%
7) Chloroethane-d5	1.571	69	142494	51.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.98%
11) 1,1-Dichloroethene-d2	2.108	63	324487	37.93	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.86%
21) 2-Butanone-d5	3.905	46	230433	93.63	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.63%
24) Chloroform-d	4.352	84	454893	46.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.037	65	361096	49.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.84%
32) Benzene-d6	5.053	84	793282	52.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.18%
36) 1,2-Dichloropropane-d6	6.076	67	196394	50.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.36%
41) Toluene-d8	7.320	98	779771	49.88	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.76%
43) trans-1,3-Dichloroprop...	7.625	79	130523	45.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.58%
47) 2-Hexanone-d5	8.095	63	159329	89.04	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.04%
56) 1,1,2,2-Tetrachloroeth...	10.223	84	279354	45.05	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.10%
66) 1,2-Dichlorobenzene-d4	11.632	152	340372	51.63	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.26%
Target Compounds						
44) trans-1,3-Dichloropropene	7.629	75	7043	0.94	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021290.D
Acq On : 05 May 2021 14:07
Operator : SY/MD
Sample : M2249-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: May 06 02:18:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 06 02:15:40 2021
Response via : Initial Calibration

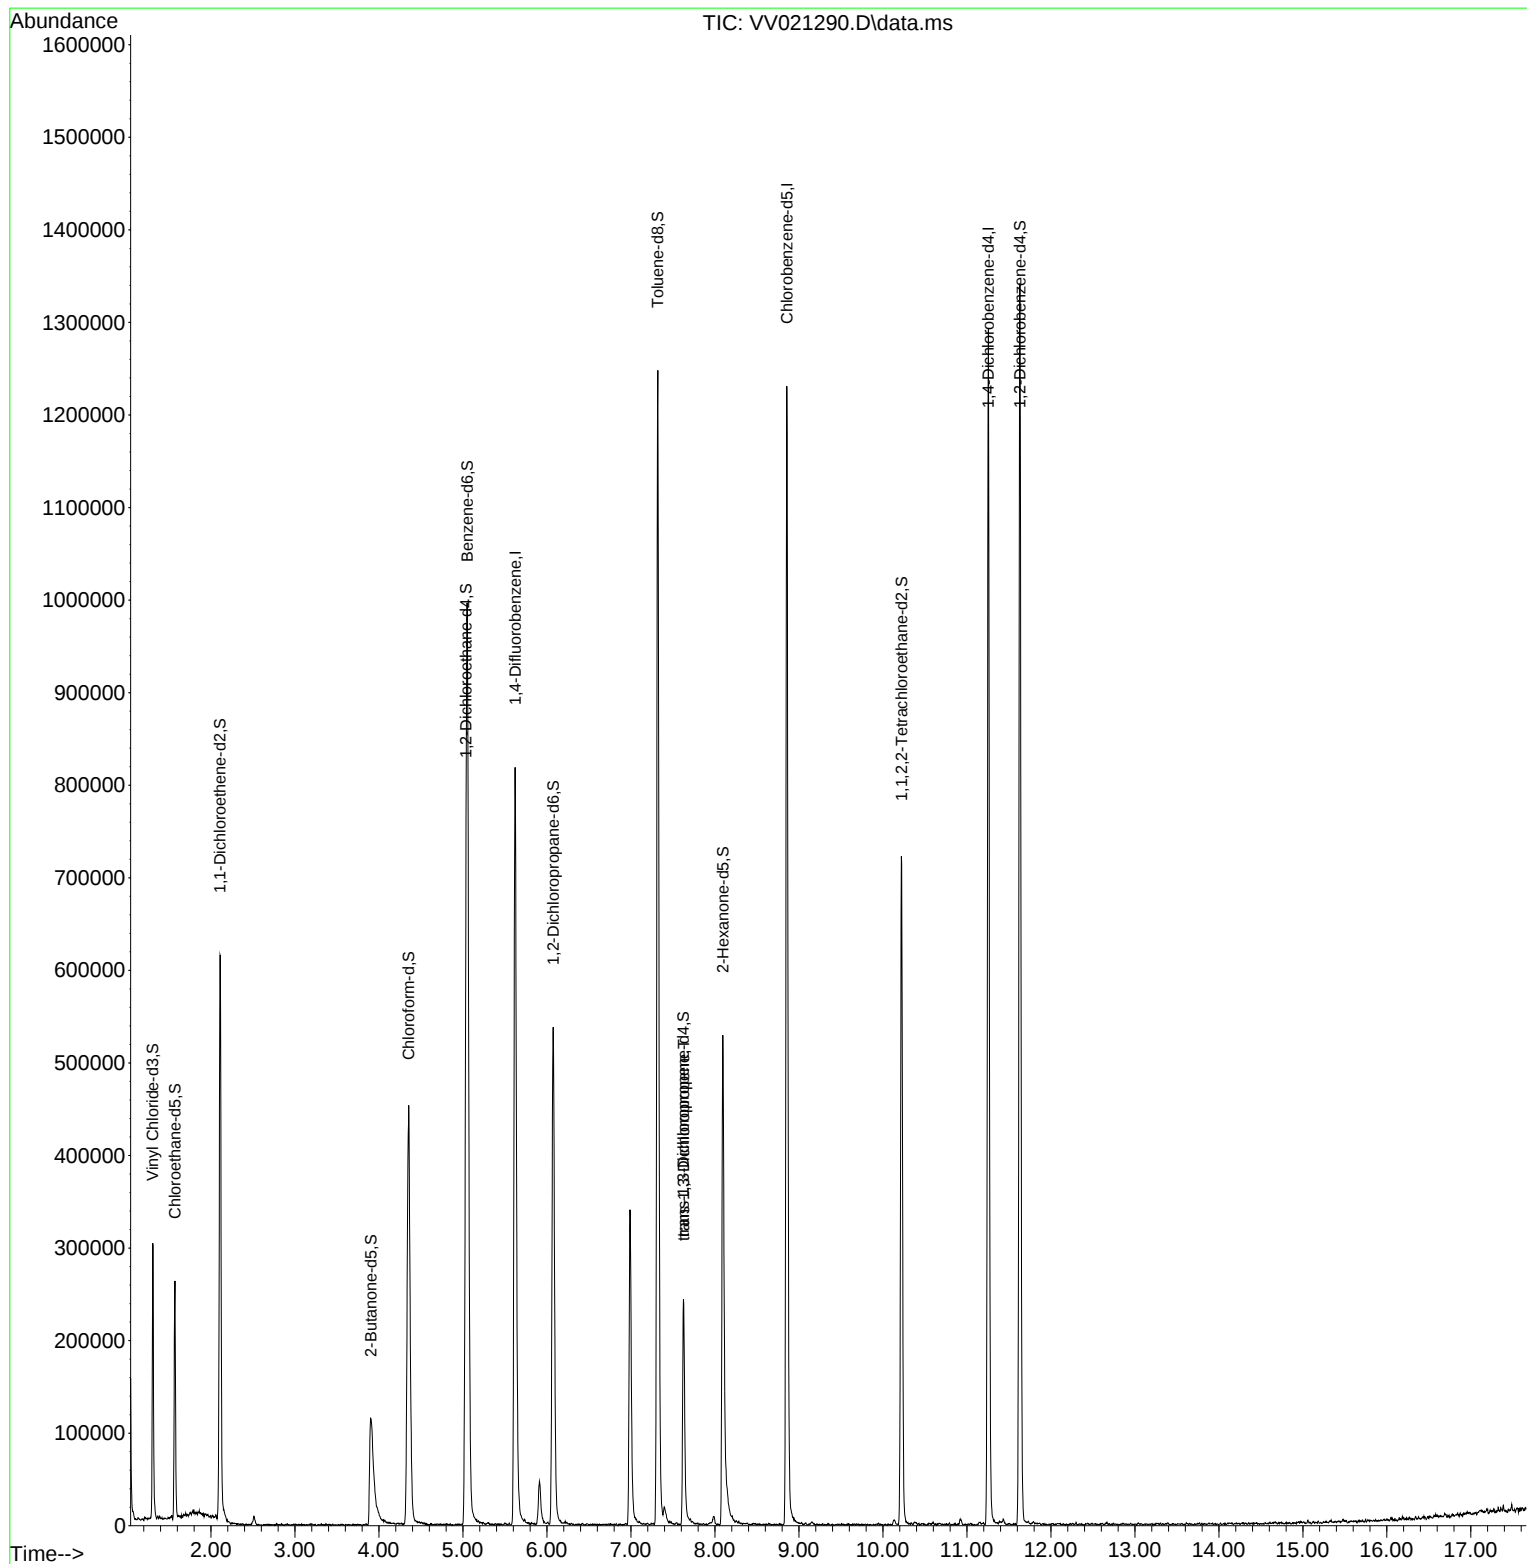

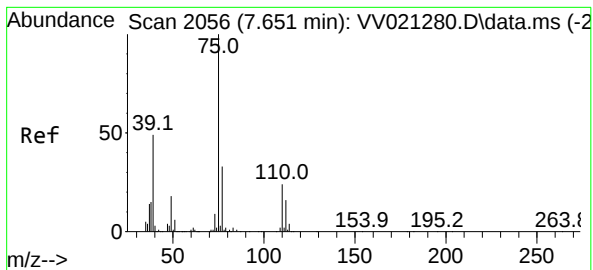

#44
 trans-1,3-Dichloropropene
 Concen: 0.94 ug/L
 RT: 7.629 min Scan# 2049
 Delta R.T. -0.022 min
 Lab File: VV021290.D
 Acq: 05 May 2021 14:07

Instrument :
 MSVOA_V
 ClientSampleId :

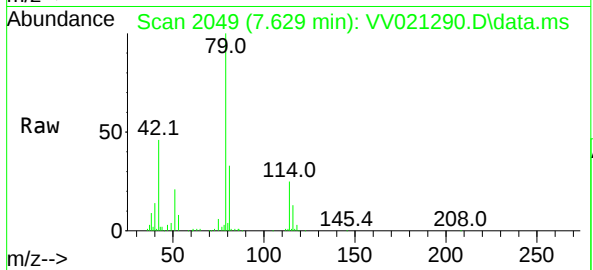

Tgt Ion: 75 Resp: 7043
 Ion Ratio Lower Upper
 75 100
 77 38.5 21.8 40.6

