

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021284.D
 Acq On : 05 May 2021 11:45
 Operator : SY/MD
 Sample : M2271-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M

Title : VOC Analysis

Signal : TIC: VV021284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	28	rVB2	34156	33524	0.73%	0.143%
2	1.310	77	84	95	rVB	189319	201974	4.40%	0.859%
3	1.571	158	165	177	rVB	195054	224407	4.88%	0.955%
4	2.108	324	332	347	rVB	452901	647926	14.10%	2.757%
5	2.423	428	430	432	rBV3	1356	732	0.02%	0.003%
6	2.461	439	442	447	rVB6	1610	1026	0.02%	0.004%
7	2.510	447	457	463	rBV10	3948	5111	0.11%	0.022%
8	2.603	484	486	489	rBV3	771	593	0.01%	0.003%
9	2.648	496	500	501	rBV3	957	605	0.01%	0.003%
10	2.773	537	539	541	rBV2	816	507	0.01%	0.002%
11	2.867	566	568	572	rVB5	1309	948	0.02%	0.004%
12	2.960	595	597	600	rBV3	910	670	0.01%	0.003%
13	3.101	640	641	643	rBV2	1047	551	0.01%	0.002%
14	3.227	677	680	684	rBV4	696	610	0.01%	0.003%
15	3.285	694	698	701	rBV3	857	821	0.02%	0.003%
16	3.339	710	715	716	rBV4	745	514	0.01%	0.002%
17	3.481	756	759	763	rBV4	1221	838	0.02%	0.004%
18	3.503	763	766	772	rBV5	1634	1454	0.03%	0.006%
19	3.580	785	790	791	rBV2	1218	1070	0.02%	0.005%
20	3.805	857	860	862	rVB4	805	484	0.01%	0.002%
21	3.863	875	878	880	rBV2	984	684	0.01%	0.003%
22	3.905	880	891	914	rBV2	121013	434514	9.46%	1.849%
23	4.291	1008	1011	1013	rBV3	1718	1005	0.02%	0.004%
24	4.352	1016	1030	1056	rVV	436733	1110469	24.17%	4.725%
25	4.728	1144	1147	1149	rVB4	1556	828	0.02%	0.004%
26	4.751	1149	1154	1157	rBV4	1293	1338	0.03%	0.006%
27	4.802	1166	1170	1171	rBV3	1459	1244	0.03%	0.005%
28	4.828	1175	1178	1181	rBV5	1177	857	0.02%	0.004%
29	4.889	1194	1197	1200	rBV4	1483	978	0.02%	0.004%
30	5.047	1230	1246	1273	rBV2	909537	2353841	51.23%	10.016%
31	5.223	1298	1301	1305	rVB4	1976	1229	0.03%	0.005%
32	5.246	1306	1308	1311	rBV2	1636	1110	0.02%	0.005%
33	5.561	1404	1406	1410	rVB4	1972	1463	0.03%	0.006%
34	5.622	1410	1425	1452	rBV	789554	1609081	35.02%	6.847%
35	5.908	1506	1514	1515	rBV3	38125	37105	0.81%	0.158%
36	6.072	1552	1565	1586	rBV	503214	1038821	22.61%	4.421%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021284.D
 Acq On : 05 May 2021 11:45
 Operator : SY/MD
 Sample : M2271-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

37	6.268	1623	1626	1629	rBV3	1972	1504	0.03%	0.006%
38	6.313	1637	1640	1641	rBV4	1013	491	0.01%	0.002%
39	6.342	1647	1649	1651	rBV3	1259	803	0.02%	0.003%
40	6.448	1680	1682	1685	rBV4	1008	567	0.01%	0.002%
41	6.471	1687	1689	1692	rVB4	1468	791	0.02%	0.003%
42	6.493	1692	1696	1697	rBV2	922	512	0.01%	0.002%
43	6.571	1718	1720	1724	rVB3	1554	911	0.02%	0.004%
44	6.674	1749	1752	1754	rBV3	1608	983	0.02%	0.004%
45	6.735	1768	1771	1773	rBV3	1881	1028	0.02%	0.004%
46	6.818	1795	1797	1803	rVB7	1123	819	0.02%	0.003%
47	6.992	1837	1851	1879	rBV2	317244	591742	12.88%	2.518%
48	7.227	1921	1924	1929	rBV6	1514	1103	0.02%	0.005%
49	7.320	1941	1953	1972	rBV	1125726	1930451	42.02%	8.215%
50	7.625	2038	2048	2060	rBV	234399	405061	8.82%	1.724%
51	7.902	2129	2134	2138	rBV6	2564	2292	0.05%	0.010%
52	7.979	2145	2158	2179	rBV	2763902	4594313	100.00%	19.551%
53	8.095	2185	2194	2227	rBV	558570	1060864	23.09%	4.514%
54	8.857	2420	2431	2450	rBV	1189999	1925517	41.91%	8.194%
55	9.143	2516	2520	2521	rBV3	2427	1655	0.04%	0.007%
56	9.349	2582	2584	2586	rBV2	1777	909	0.02%	0.004%
57	9.471	2619	2622	2625	rBV3	1951	1176	0.03%	0.005%
58	9.506	2630	2633	2636	rVV5	1241	821	0.02%	0.003%
59	9.648	2675	2677	2681	rBV4	958	692	0.02%	0.003%
60	9.734	2702	2704	2706	rVB3	1405	584	0.01%	0.002%
61	9.751	2706	2709	2711	rBV2	1166	543	0.01%	0.002%
62	9.815	2725	2729	2731	rBV2	1489	827	0.02%	0.004%
63	9.902	2753	2756	2761	rVB5	2757	2147	0.05%	0.009%
64	9.947	2767	2770	2773	rBV3	901	650	0.01%	0.003%
65	10.005	2784	2788	2789	rBV3	697	584	0.01%	0.002%
66	10.046	2798	2801	2803	rBV4	1125	505	0.01%	0.002%
67	10.062	2803	2806	2811	rBV6	1521	1155	0.03%	0.005%
68	10.220	2844	2855	2877	rBV2	767096	1233913	26.86%	5.251%
69	10.387	2904	2907	2913	rVB7	3291	3381	0.07%	0.014%
70	10.426	2918	2919	2923	rVB3	1860	864	0.02%	0.004%
71	10.593	2969	2971	2973	rBV3	1248	681	0.01%	0.003%
72	10.651	2987	2989	2992	rBV2	1796	1103	0.02%	0.005%
73	10.895	3061	3065	3067	rBV5	2148	1496	0.03%	0.006%
74	10.921	3070	3073	3087	rVB5	6120	9392	0.20%	0.040%
75	11.040	3105	3110	3113	rBV7	1725	2167	0.05%	0.009%
76	11.255	3164	3177	3195	rBV2	1216089	1915802	41.70%	8.152%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021284.D
 Acq On : 05 May 2021 11:45
 Operator : SY/MD
 Sample : M2271-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M

Title : VOC Analysis

77	11.632	3282	3294	3317	rBV	1301002	2052670	44.68%	8.735%
78	11.876	3368	3370	3373	rVB4	1491	588	0.01%	0.003%
79	11.895	3373	3376	3379	rBV3	1091	641	0.01%	0.003%
80	11.956	3393	3395	3397	rBV2	1018	518	0.01%	0.002%
81	12.008	3408	3411	3415	rVB3	2026	1340	0.03%	0.006%
82	12.040	3415	3421	3423	rBV5	1781	1828	0.04%	0.008%
83	12.078	3431	3433	3435	rBV3	1238	772	0.02%	0.003%
84	12.127	3445	3448	3450	rVB4	1294	646	0.01%	0.003%
85	12.246	3482	3485	3488	rBV3	1762	1430	0.03%	0.006%
86	12.419	3536	3539	3541	rVB4	1374	889	0.02%	0.004%
87	12.545	3575	3578	3579	rBV2	1047	565	0.01%	0.002%
88	12.577	3585	3588	3591	rBV3	1571	1223	0.03%	0.005%
89	12.757	3639	3644	3649	rBV6	2052	1948	0.04%	0.008%
90	12.795	3654	3656	3658	rBV3	1259	802	0.02%	0.003%
91	12.908	3689	3691	3693	rBV3	1205	730	0.02%	0.003%
92	13.062	3737	3739	3742	rBV5	1434	829	0.02%	0.004%
93	13.496	3872	3874	3879	rBV5	1487	1032	0.02%	0.004%
94	13.766	3956	3958	3962	rBV2	931	506	0.01%	0.002%
95	13.892	3995	3997	4001	rVB3	1567	845	0.02%	0.004%
96	14.123	4067	4069	4077	rVB7	2587	2762	0.06%	0.012%
97	14.165	4077	4082	4085	rBV4	2705	2538	0.06%	0.011%
98	14.220	4096	4099	4101	rBV4	2243	1007	0.02%	0.004%
99	14.307	4122	4126	4129	rBV4	2629	2338	0.05%	0.010%
100	14.461	4171	4174	4178	rBV4	1574	1486	0.03%	0.006%




Sum of corrected areas: 23499664

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021284.D
Acq On : 05 May 2021 11:45
Operator : SY/MD
Sample : M2271-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

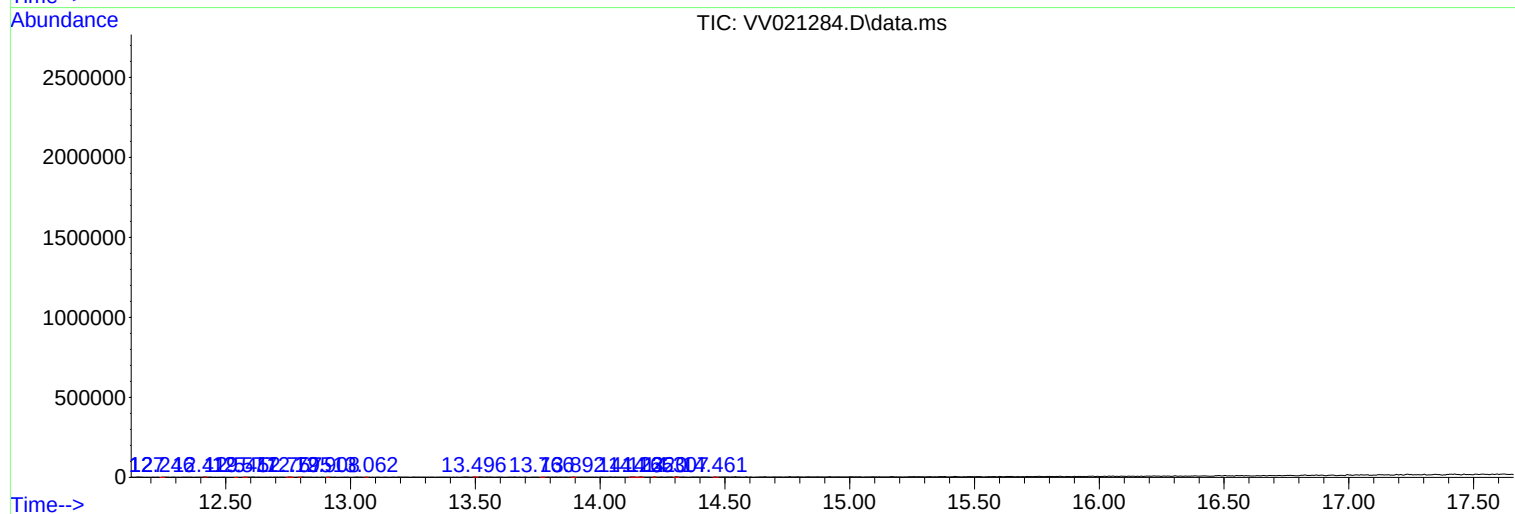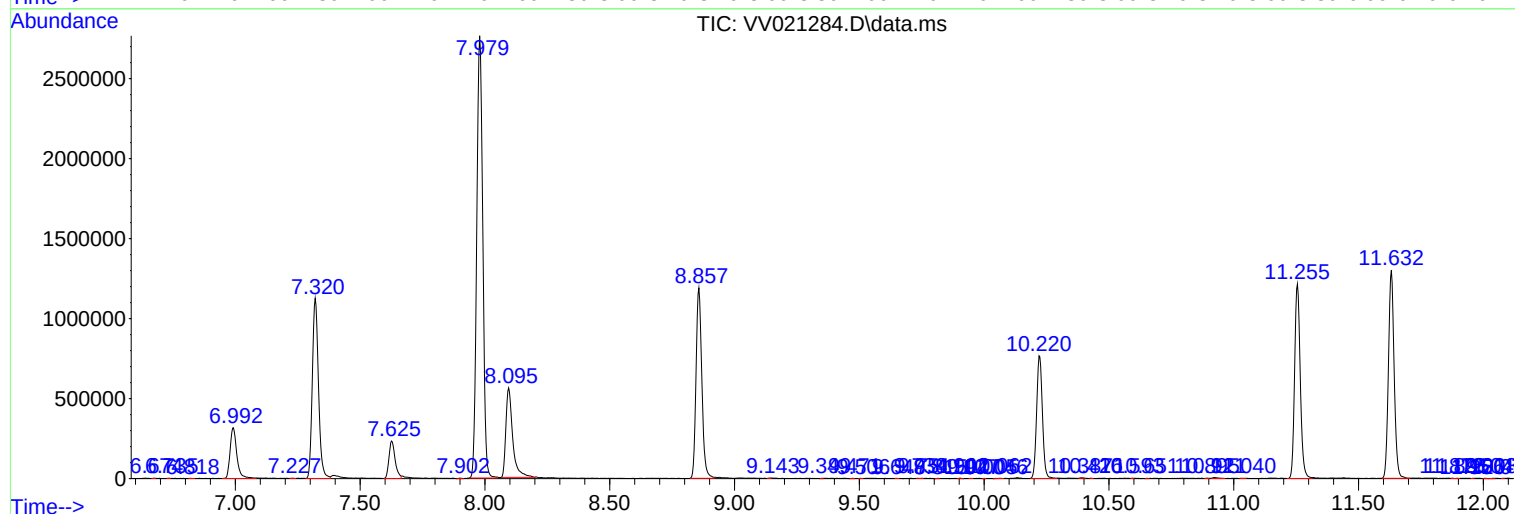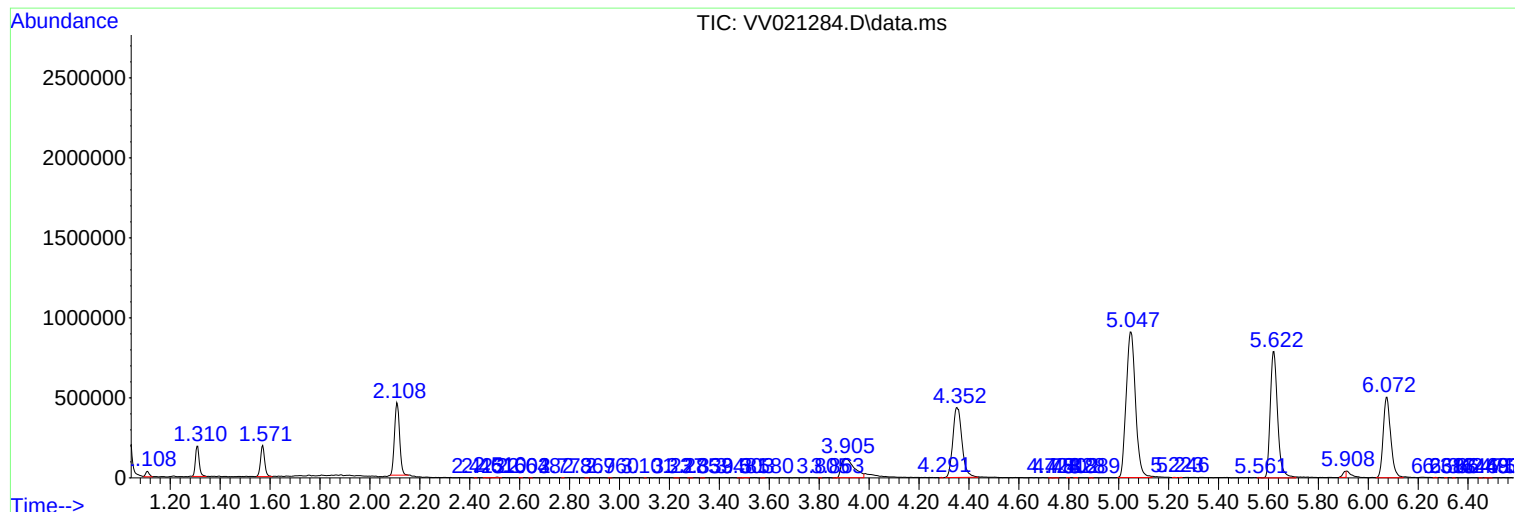

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021284.D
Acq On : 05 May 2021 11:45
Operator : SY/MD
Sample : M2271-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021284.D
Acq On : 05 May 2021 11:45
Operator : SY/MD
Sample : M2271-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
