

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V050521\
 Data File : V021291.D
 Acq On : 05 May 2021 14:30
 Operator : SY/MD
 Sample : M2271-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

Signal : TIC: V021291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rBV	176408	175193	8.11%	0.877%
2	1.568	157	164	173	rBV	177661	205343	9.51%	1.028%
3	2.108	323	332	345	rBV	423900	615382	28.50%	3.080%
4	2.436	430	434	438	rBV5	1474	1631	0.08%	0.008%
5	2.458	438	441	442	rBV2	1403	903	0.04%	0.005%
6	2.513	450	458	469	rVB6	11529	18727	0.87%	0.094%
7	2.571	473	476	482	rVB4	1184	995	0.05%	0.005%
8	2.597	482	484	487	rBV3	1026	707	0.03%	0.004%
9	2.696	507	515	518	rVB7	1386	1632	0.08%	0.008%
10	2.735	524	527	532	rBV5	993	816	0.04%	0.004%
11	2.802	544	548	549	rBV2	1751	1156	0.05%	0.006%
12	2.905	577	580	583	rBV3	1111	725	0.03%	0.004%
13	2.957	593	596	600	rVB5	1282	951	0.04%	0.005%
14	3.011	609	613	621	rVB6	1062	1274	0.06%	0.006%
15	3.069	628	631	633	rVB3	1372	808	0.04%	0.004%
16	3.140	651	653	658	rBV6	1620	1173	0.05%	0.006%
17	3.262	688	691	696	rBV6	897	872	0.04%	0.004%
18	3.320	707	709	710	rBV	1491	708	0.03%	0.004%
19	3.368	721	724	728	rBV6	1143	1008	0.05%	0.005%
20	3.436	741	745	746	rBV2	1191	674	0.03%	0.003%
21	3.552	777	781	786	rVB3	1048	847	0.04%	0.004%
22	3.638	805	808	812	rBV4	1142	858	0.04%	0.004%
23	3.674	814	819	824	rBV5	722	867	0.04%	0.004%
24	3.719	830	833	835	rBV2	1304	729	0.03%	0.004%
25	3.844	870	872	876	rVB4	1623	1021	0.05%	0.005%
26	3.902	876	890	919	rBV	124110	446286	20.67%	2.234%
27	4.294	1008	1012	1014	rBV4	1897	1554	0.07%	0.008%
28	4.352	1014	1030	1056	rVV	413902	981616	45.46%	4.913%
29	4.529	1082	1085	1090	rVB6	2128	1437	0.07%	0.007%
30	4.580	1098	1101	1104	rBV3	1435	1220	0.06%	0.006%
31	4.654	1120	1124	1127	rBV3	1712	1249	0.06%	0.006%
32	4.712	1139	1142	1144	rBV2	1100	736	0.03%	0.004%
33	4.761	1152	1157	1159	rBV4	1160	1003	0.05%	0.005%
34	4.799	1165	1169	1170	rBV3	1226	734	0.03%	0.004%
35	4.854	1183	1186	1189	rBV3	2690	1942	0.09%	0.010%
36	4.934	1209	1211	1214	rBV3	1237	822	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021291.D
 Acq On : 05 May 2021 14:30
 Operator : SY/MD
 Sample : M2271-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

37	4.973	1219	1223	1225	rBV4	1179	888	0.04%	0.004%
38	5.050	1230	1247	1275	rBV3	839587	2159272	100.00%	10.807%
39	5.619	1412	1424	1454	rBV	818107	1655953	76.69%	8.288%
40	5.912	1503	1515	1533	rBV3	46441	104322	4.83%	0.522%
41	6.076	1549	1566	1588	rBV3	461562	968166	44.84%	4.846%
42	6.378	1656	1660	1663	rBV4	1067	896	0.04%	0.004%
43	6.613	1730	1733	1735	rBV3	1210	720	0.03%	0.004%
44	6.722	1765	1767	1770	rBV3	936	680	0.03%	0.003%
45	6.818	1792	1797	1798	rBV	1366	1052	0.05%	0.005%
46	6.918	1821	1828	1830	rBV8	1866	1950	0.09%	0.010%
47	6.992	1839	1851	1876	rBV	295217	550146	25.48%	2.753%
48	7.188	1907	1912	1917	rBV8	2812	3064	0.14%	0.015%
49	7.320	1941	1953	1969	rBV	993047	1724175	79.85%	8.629%
50	7.506	2007	2011	2012	rBV3	2259	1581	0.07%	0.008%
51	7.625	2038	2048	2071	rBV	202263	372544	17.25%	1.865%
52	7.889	2128	2130	2134	rBV3	1686	1199	0.06%	0.006%
53	7.921	2137	2140	2142	rBV3	1546	1089	0.05%	0.005%
54	7.979	2146	2158	2180	rVV	1104922	1825833	84.56%	9.138%
55	8.095	2185	2194	2231	rVV2	520025	1028585	47.64%	5.148%
56	8.532	2327	2330	2332	rBV2	1651	806	0.04%	0.004%
57	8.567	2339	2341	2347	rVB4	1819	1540	0.07%	0.008%
58	8.619	2353	2357	2359	rBV3	1901	1364	0.06%	0.007%
59	8.651	2364	2367	2370	rBV3	2255	1482	0.07%	0.007%
60	8.857	2420	2431	2457	rVV	1241948	2023672	93.72%	10.128%
61	9.079	2497	2500	2501	rBV2	1832	1071	0.05%	0.005%
62	9.188	2533	2534	2541	rVB4	2015	1742	0.08%	0.009%
63	9.223	2541	2545	2548	rBV4	1015	891	0.04%	0.004%
64	9.246	2548	2552	2555	rBV4	1082	1115	0.05%	0.006%
65	9.368	2588	2590	2593	rVB4	1696	854	0.04%	0.004%
66	9.558	2644	2649	2655	rBV7	1582	1978	0.09%	0.010%
67	9.699	2690	2693	2696	rBV5	1221	771	0.04%	0.004%
68	9.731	2701	2703	2705	rBV3	1300	692	0.03%	0.003%
69	9.889	2748	2752	2755	rVV5	1377	1043	0.05%	0.005%
70	9.934	2762	2766	2769	rBV5	1681	1404	0.07%	0.007%
71	10.066	2804	2807	2809	rBV3	1180	762	0.04%	0.004%
72	10.098	2814	2817	2821	rBV3	1209	1116	0.05%	0.006%
73	10.178	2839	2842	2843	rBV2	1318	665	0.03%	0.003%
74	10.223	2843	2856	2875	rVV2	729363	1159209	53.69%	5.802%
75	10.452	2924	2927	2932	rBV6	1919	1281	0.06%	0.006%
76	10.477	2932	2935	2937	rBV3	1297	861	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021291.D
 Acq On : 05 May 2021 14:30
 Operator : SY/MD
 Sample : M2271-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M

Title : VOC Analysis

77	10.600	2969	2973	2976	rBV5	1887	1529	0.07%	0.008%
78	10.674	2991	2996	3002	rVB8	1878	2237	0.10%	0.011%
79	10.870	3054	3057	3060	rBV3	1899	1062	0.05%	0.005%
80	11.053	3109	3114	3115	rBV3	1349	1020	0.05%	0.005%
81	11.130	3133	3138	3140	rBV4	2236	1849	0.09%	0.009%
82	11.255	3166	3177	3196	rBV	1290225	1999193	92.59%	10.006%
83	11.632	3280	3294	3312	rBV	1198124	1873050	86.74%	9.375%
84	11.847	3359	3361	3364	rBV4	1720	964	0.04%	0.005%
85	11.889	3372	3374	3378	rBV6	1280	818	0.04%	0.004%
86	12.188	3464	3467	3469	rBV2	1852	1128	0.05%	0.006%
87	12.236	3479	3482	3486	rVB5	1518	1106	0.05%	0.006%
88	12.342	3512	3515	3516	rBV	1461	670	0.03%	0.003%
89	12.612	3596	3599	3602	rBV4	1555	987	0.05%	0.005%
90	12.712	3628	3630	3633	rBV3	1508	1212	0.06%	0.006%
91	12.757	3640	3644	3648	rBV6	1062	1002	0.05%	0.005%
92	12.780	3648	3651	3654	rVV3	1804	1015	0.05%	0.005%
93	12.812	3658	3661	3666	rVB	4255	2784	0.13%	0.014%
94	12.985	3712	3715	3719	rBV6	1483	1202	0.06%	0.006%
95	13.165	3768	3771	3773	rBV3	1045	831	0.04%	0.004%
96	13.275	3802	3805	3809	rBV5	2373	1914	0.09%	0.010%
97	13.677	3927	3930	3935	rBV5	1197	1140	0.05%	0.006%
98	13.722	3941	3944	3947	rBV4	1845	1227	0.06%	0.006%
99	14.095	4057	4060	4064	rBV3	1593	1012	0.05%	0.005%
100	14.841	4290	4292	4294	rBV2	2083	1062	0.05%	0.005%


Sum of corrected areas: 19980047

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021291.D
Acq On : 05 May 2021 14:30
Operator : SY/MD
Sample : M2271-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

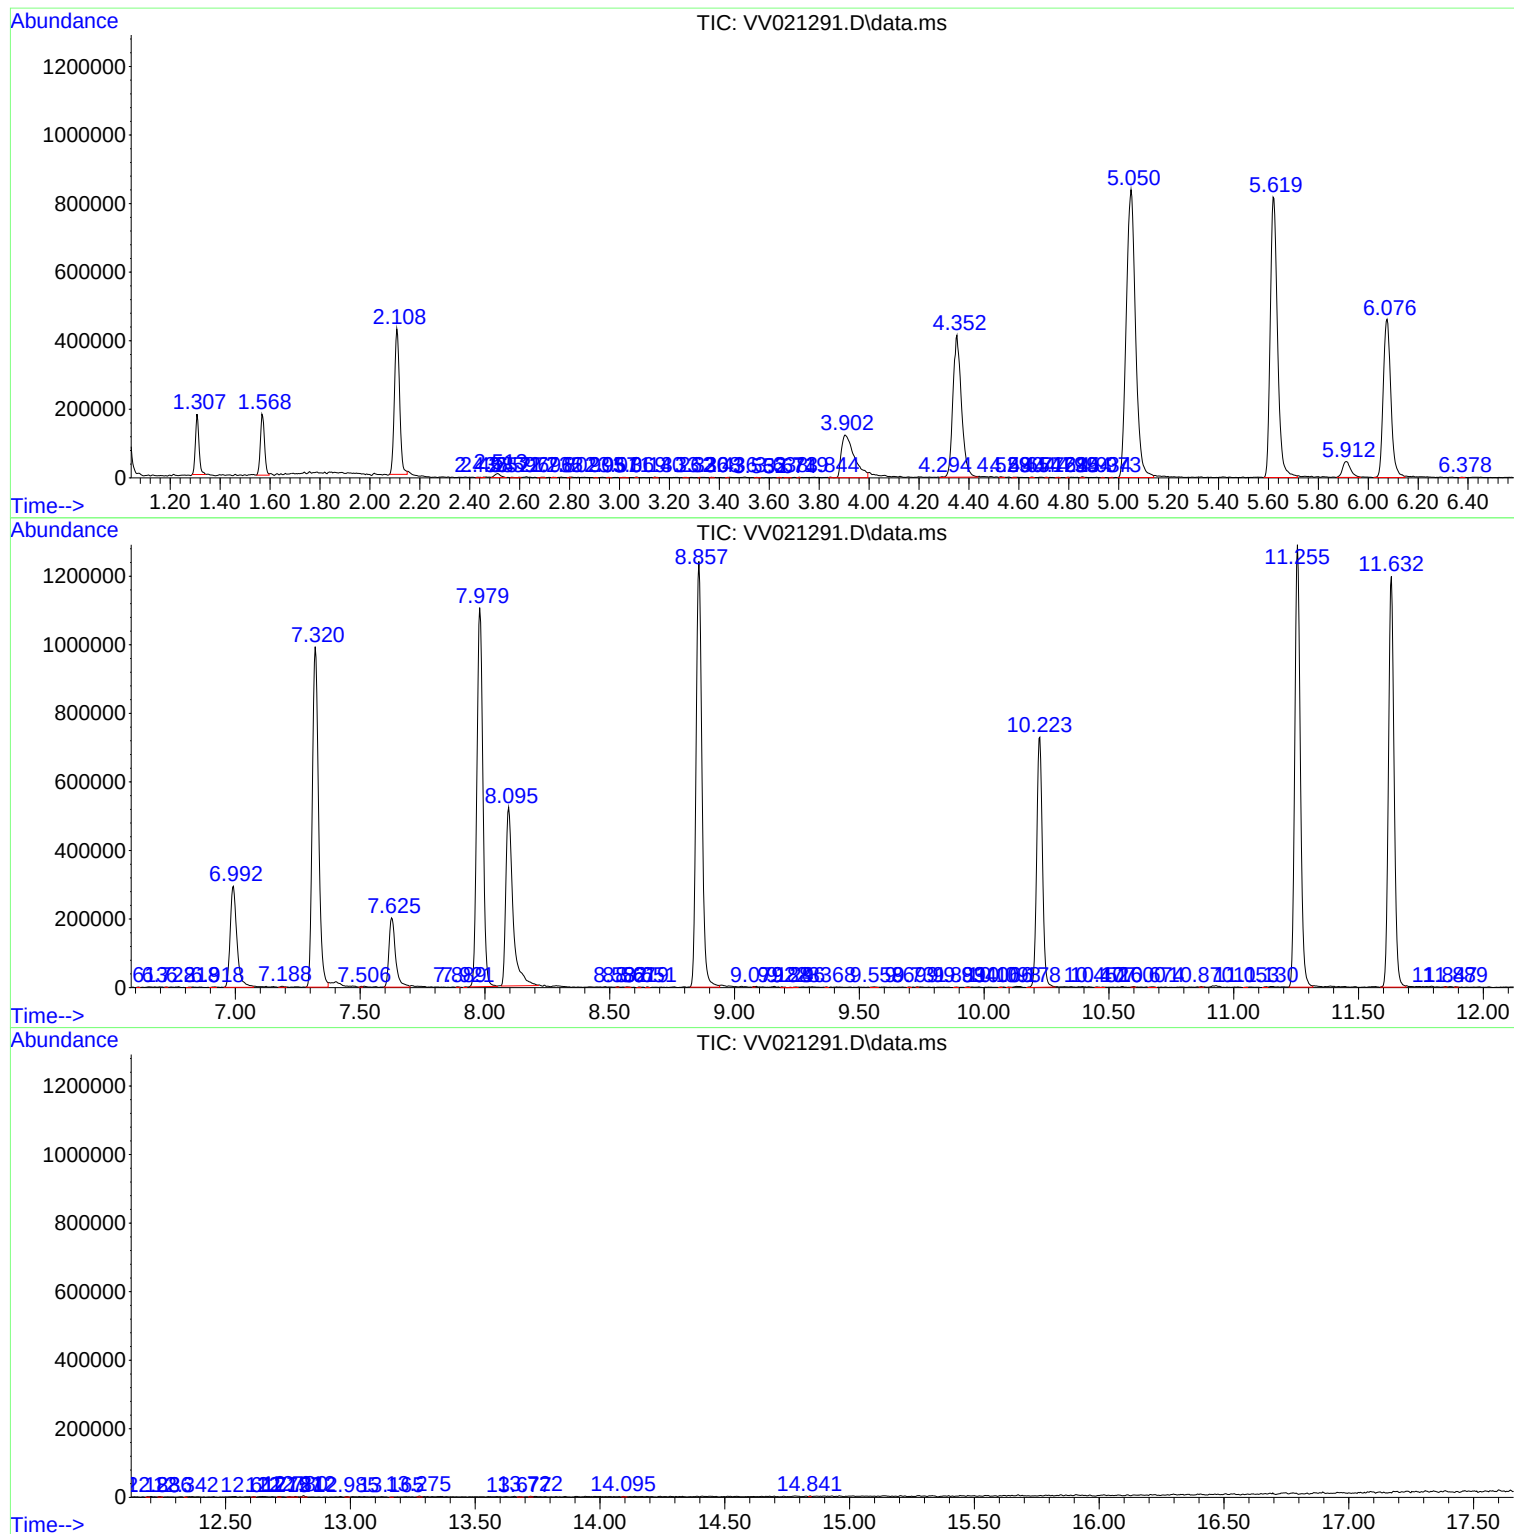

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021291.D
Acq On : 05 May 2021 14:30
Operator : SY/MD
Sample : M2271-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021291.D
Acq On : 05 May 2021 14:30
Operator : SY/MD
Sample : M2271-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
