

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V050521\
 Data File : V021295.D
 Acq On : 05 May 2021 16:05
 Operator : SY/MD
 Sample : M2271-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M

Title : VOC Analysis

Signal : TIC: V021295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	92	rBV	139230	142659	6.79%	0.782%
2	1.568	158	164	175	rVB	148283	172118	8.20%	0.944%
3	2.108	324	332	353	rVB	365702	540449	25.73%	2.964%
4	2.433	429	433	434	rBV2	1184	719	0.03%	0.004%
5	2.497	451	453	454	rBV2	2421	1025	0.05%	0.006%
6	2.748	527	531	534	rBV4	1515	1009	0.05%	0.006%
7	2.857	562	565	567	rBV3	1312	682	0.03%	0.004%
8	2.963	593	598	600	rBV4	1772	1698	0.08%	0.009%
9	3.014	611	614	617	rVB3	1230	726	0.03%	0.004%
10	3.034	617	620	623	rBV2	1489	1030	0.05%	0.006%
11	3.050	623	625	630	rBV4	958	900	0.04%	0.005%
12	3.198	669	671	674	rVB3	1828	1059	0.05%	0.006%
13	3.214	674	676	681	rVB4	994	900	0.04%	0.005%
14	3.243	681	685	689	rBV6	983	919	0.04%	0.005%
15	3.407	732	736	739	rVB5	1363	1063	0.05%	0.006%
16	3.429	739	743	745	rBV3	1883	1237	0.06%	0.007%
17	3.484	758	760	764	rBV3	1468	1142	0.05%	0.006%
18	3.715	830	832	834	rBV2	1506	734	0.03%	0.004%
19	3.773	845	850	853	rVB5	1155	932	0.04%	0.005%
20	3.908	878	892	914	rBV2	101379	369293	17.58%	2.025%
21	4.178	974	976	979	rVB3	1928	990	0.05%	0.005%
22	4.352	1014	1030	1049	rBV2	337185	827203	39.39%	4.537%
23	4.561	1093	1095	1100	rVB5	1685	1237	0.06%	0.007%
24	4.683	1130	1133	1135	rVV4	1567	984	0.05%	0.005%
25	4.696	1135	1137	1140	rVB3	1372	680	0.03%	0.004%
26	4.728	1145	1147	1155	rVB7	1975	1737	0.08%	0.010%
27	4.764	1155	1158	1162	rBV4	1544	1415	0.07%	0.008%
28	4.921	1203	1207	1209	rVV4	1091	940	0.04%	0.005%
29	4.947	1212	1215	1217	rVB4	1670	822	0.04%	0.005%
30	5.050	1230	1247	1270	rBV3	682207	1804599	85.93%	9.897%
31	5.297	1321	1324	1326	rBV2	1440	916	0.04%	0.005%
32	5.368	1343	1346	1348	rVV3	1239	796	0.04%	0.004%
33	5.455	1369	1373	1375	rBV3	1265	967	0.05%	0.005%
34	5.558	1402	1405	1408	rBV2	1519	1189	0.06%	0.007%
35	5.619	1413	1424	1452	rVV	867559	1735190	82.62%	9.517%
36	5.915	1506	1516	1528	rBV5	34882	71920	3.42%	0.394%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021295.D
 Acq On : 05 May 2021 16:05
 Operator : SY/MD
 Sample : M2271-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

37	6.075	1553	1566	1588	rBV2	389649	803235	38.25%	4.405%
38	6.214	1605	1609	1611	rBV4	2158	1891	0.09%	0.010%
39	6.352	1650	1652	1656	rVV2	1297	979	0.05%	0.005%
40	6.445	1678	1681	1683	rBV3	1270	902	0.04%	0.005%
41	6.510	1697	1701	1705	rBV4	1217	1041	0.05%	0.006%
42	6.535	1705	1709	1712	rBV4	2392	1532	0.07%	0.008%
43	6.577	1720	1722	1727	rVB4	1371	1161	0.06%	0.006%
44	6.873	1812	1814	1819	rBV5	1744	1280	0.06%	0.007%
45	6.992	1840	1851	1869	rBV2	239961	444188	21.15%	2.436%
46	7.204	1913	1917	1924	rBV7	1695	2046	0.10%	0.011%
47	7.265	1934	1936	1939	rBV4	1858	1049	0.05%	0.006%
48	7.320	1942	1953	1973	rBV	820523	1418485	67.54%	7.780%
49	7.628	2039	2049	2072	rBV2	163541	302909	14.42%	1.661%
50	7.854	2114	2119	2120	rBV4	1248	948	0.05%	0.005%
51	7.979	2143	2158	2178	rBV	1116738	1861500	88.64%	10.209%
52	8.095	2184	2194	2226	rBV2	445630	900618	42.88%	4.939%
53	8.387	2282	2285	2287	rBV3	1849	971	0.05%	0.005%
54	8.542	2327	2333	2337	rBV6	1545	2234	0.11%	0.012%
55	8.571	2340	2342	2344	rBV3	1611	780	0.04%	0.004%
56	8.815	2416	2418	2420	rBV2	1526	887	0.04%	0.005%
57	8.857	2420	2431	2450	rBV	1309844	2100151	100.00%	11.518%
58	9.172	2527	2529	2531	rBV4	1507	844	0.04%	0.005%
59	9.278	2557	2562	2565	rBV5	1641	1646	0.08%	0.009%
60	9.593	2658	2660	2666	rBV5	1017	911	0.04%	0.005%
61	9.619	2666	2668	2673	rVB5	1202	785	0.04%	0.004%
62	9.911	2757	2759	2762	rBV3	1266	833	0.04%	0.005%
63	9.998	2784	2786	2792	rVB6	1047	834	0.04%	0.005%
64	10.027	2792	2795	2799	rBV4	2018	1515	0.07%	0.008%
65	10.085	2810	2813	2815	rBV3	1298	884	0.04%	0.005%
66	10.114	2818	2822	2824	rBV4	976	837	0.04%	0.005%
67	10.130	2824	2827	2829	rBV3	1693	1390	0.07%	0.008%
68	10.223	2843	2856	2876	rBV2	637180	995540	47.40%	5.460%
69	10.381	2902	2905	2907	rBV3	1986	1180	0.06%	0.006%
70	10.496	2937	2941	2942	rBV2	1126	719	0.03%	0.004%
71	10.558	2956	2960	2964	rBV5	1657	1385	0.07%	0.008%
72	10.580	2964	2967	2972	rVV6	1721	1517	0.07%	0.008%
73	10.615	2975	2978	2983	rVB6	1533	1069	0.05%	0.006%
74	10.834	3041	3046	3049	rBV5	1880	1649	0.08%	0.009%
75	11.043	3107	3111	3119	rVB8	1971	1776	0.08%	0.010%
76	11.088	3120	3125	3132	rBV9	1894	2838	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V050521\
 Data File : V021295.D
 Acq On : 05 May 2021 16:05
 Operator : SY/MD
 Sample : M2271-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

77	11.255	3165	3177	3196	rBV	1330410	2080301	99.05%	11.409%
78	11.506	3251	3255	3261	rBV5	2231	2389	0.11%	0.013%
79	11.631	3282	3294	3308	rBV	977565	1568538	74.69%	8.603%
80	11.840	3357	3359	3362	rBV3	1196	764	0.04%	0.004%
81	11.992	3403	3406	3411	rVB3	1410	927	0.04%	0.005%
82	12.049	3421	3424	3427	rVB3	1206	700	0.03%	0.004%
83	12.072	3427	3431	3435	rBV5	1141	1237	0.06%	0.007%
84	12.123	3443	3447	3451	rBV7	1584	1602	0.08%	0.009%
85	12.310	3501	3505	3507	rBV3	1584	1152	0.05%	0.006%
86	12.419	3536	3539	3541	rBV2	1396	1007	0.05%	0.006%
87	12.461	3548	3552	3554	rBV4	1430	998	0.05%	0.005%
88	12.599	3590	3595	3596	rBV3	2190	1656	0.08%	0.009%
89	12.676	3617	3619	3627	rVB7	1495	966	0.05%	0.005%
90	12.789	3650	3654	3657	rBV5	1477	1190	0.06%	0.007%
91	12.995	3715	3718	3721	rBV5	1333	807	0.04%	0.004%
92	13.014	3721	3724	3727	rBV2	1362	762	0.04%	0.004%
93	13.056	3735	3737	3741	rVB5	1620	887	0.04%	0.005%
94	13.236	3790	3793	3795	rBV2	1342	712	0.03%	0.004%
95	13.281	3804	3807	3809	rBV3	1405	1034	0.05%	0.006%
96	13.419	3846	3850	3854	rBV4	1667	1766	0.08%	0.010%
97	13.519	3878	3881	3886	rVB4	2646	2000	0.10%	0.011%
98	13.551	3887	3891	3894	rBV5	1584	1239	0.06%	0.007%
99	14.107	4061	4064	4067	rBV4	1075	762	0.04%	0.004%
100	14.725	4254	4256	4258	rBV2	1826	1036	0.05%	0.006%


Sum of corrected areas: 18233250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021295.D
Acq On : 05 May 2021 16:05
Operator : SY/MD
Sample : M2271-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

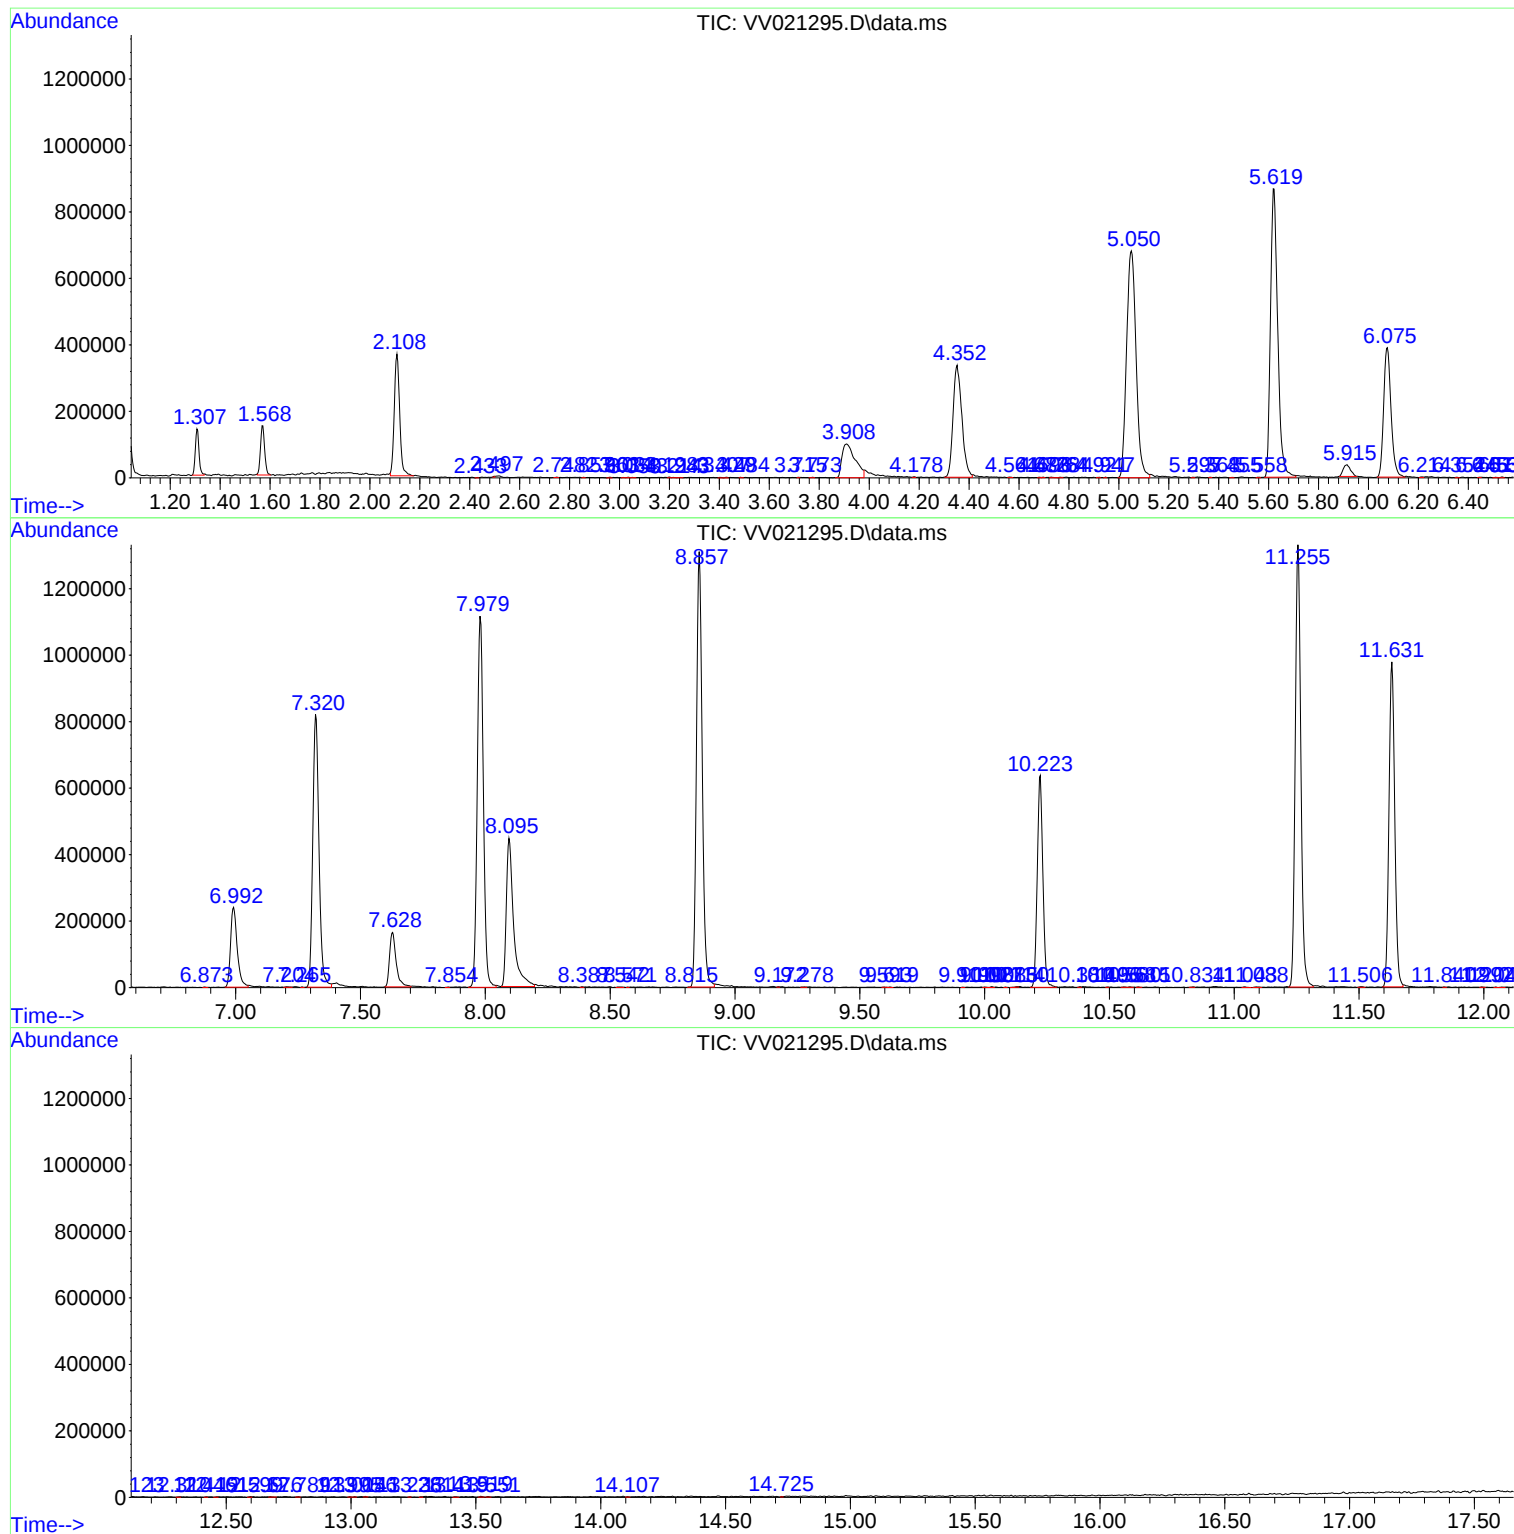

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021295.D
Acq On : 05 May 2021 16:05
Operator : SY/MD
Sample : M2271-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021295.D
Acq On : 05 May 2021 16:05
Operator : SY/MD
Sample : M2271-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
