

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V050521\
 Data File : VV021296.D
 Acq On : 05 May 2021 16:28
 Operator : SY/MD
 Sample : M2271-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M

Title : VOC Analysis

Signal : TIC: VV021296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	165923	169138	8.18%	0.968%
2	1.571	158	165	177	rVB	164056	183949	8.90%	1.052%
3	2.108	323	332	354	rVB	406051	596973	28.88%	3.416%
4	2.359	407	410	416	rVB7	1522	1358	0.07%	0.008%
5	2.401	420	423	427	rVB6	1544	881	0.04%	0.005%
6	2.433	430	433	438	rVB5	2040	1542	0.07%	0.009%
7	2.458	438	441	445	rBV4	2340	1796	0.09%	0.010%
8	2.542	464	467	472	rVB6	1649	1283	0.06%	0.007%
9	2.568	472	475	479	rBV3	1454	977	0.05%	0.006%
10	2.590	479	482	485	rBV4	1079	800	0.04%	0.005%
11	2.610	485	488	490	rBV3	1536	983	0.05%	0.006%
12	2.757	529	534	538	rBV8	1966	2332	0.11%	0.013%
13	2.780	538	541	545	rBV4	2316	1464	0.07%	0.008%
14	2.835	554	558	560	rBV4	1551	1067	0.05%	0.006%
15	2.896	573	577	581	rBV5	1361	807	0.04%	0.005%
16	2.921	581	585	588	rBV4	1580	1058	0.05%	0.006%
17	2.966	597	599	605	rVB3	1291	1086	0.05%	0.006%
18	2.999	605	609	612	rBV4	999	818	0.04%	0.005%
19	3.040	620	622	626	rBV4	2243	1746	0.08%	0.010%
20	3.330	710	712	720	rBV6	954	1043	0.05%	0.006%
21	3.375	723	726	730	rVB3	1471	951	0.05%	0.005%
22	3.397	730	733	736	rBV3	2048	1300	0.06%	0.007%
23	3.455	746	751	752	rBV3	1186	925	0.04%	0.005%
24	3.516	767	770	773	rVB3	1259	786	0.04%	0.004%
25	3.687	819	823	825	rVV3	1018	831	0.04%	0.005%
26	3.767	846	848	853	rVB5	1516	766	0.04%	0.004%
27	3.905	879	891	918	rBV	111724	387253	18.74%	2.216%
28	4.246	991	997	999	rBV4	973	1043	0.05%	0.006%
29	4.352	1015	1030	1053	rBV2	388842	956992	46.30%	5.475%
30	4.651	1121	1123	1125	rVV2	1775	885	0.04%	0.005%
31	4.690	1129	1135	1138	rBV6	1301	1446	0.07%	0.008%
32	4.744	1149	1152	1155	rBV4	1127	837	0.04%	0.005%
33	4.883	1192	1195	1197	rBV3	1101	712	0.03%	0.004%
34	4.966	1216	1221	1226	rVB5	2141	1951	0.09%	0.011%
35	5.050	1228	1247	1273	rBV4	757674	1992822	96.41%	11.402%
36	5.352	1339	1341	1344	rVB4	1935	983	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021296.D
 Acq On : 05 May 2021 16:28
 Operator : SY/MD
 Sample : M2271-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

37	5.371	1344	1347	1352	rVB6	1781	1312	0.06%	0.008%
38	5.503	1386	1388	1392	rVB4	1625	1145	0.06%	0.007%
39	5.526	1392	1395	1399	rBV4	1553	1227	0.06%	0.007%
40	5.619	1412	1424	1449	rBV2	831927	1682641	81.41%	9.627%
41	5.796	1477	1479	1484	rVB4	1961	1052	0.05%	0.006%
42	5.912	1500	1515	1529	rBV5	35275	82813	4.01%	0.474%
43	6.076	1552	1566	1587	rBV2	438038	895912	43.34%	5.126%
44	6.310	1636	1639	1642	rBV4	1543	1162	0.06%	0.007%
45	6.484	1690	1693	1697	rBV6	1117	962	0.05%	0.006%
46	6.529	1701	1707	1708	rBV4	955	833	0.04%	0.005%
47	6.635	1736	1740	1742	rBV5	1834	1523	0.07%	0.009%
48	6.744	1772	1774	1778	rBV4	1129	947	0.05%	0.005%
49	6.860	1804	1810	1813	rBV6	1201	1198	0.06%	0.007%
50	6.992	1840	1851	1876	rVV2	267409	505168	24.44%	2.890%
51	7.137	1893	1896	1899	rVB4	2437	1669	0.08%	0.010%
52	7.211	1917	1919	1924	rBV5	2090	1834	0.09%	0.010%
53	7.320	1941	1953	1970	rBV	908641	1570024	75.96%	8.983%
54	7.625	2038	2048	2068	rBV2	204554	352417	17.05%	2.016%
55	7.918	2134	2139	2141	rBV4	2540	2168	0.10%	0.012%
56	8.095	2184	2194	2222	rBV2	499923	985376	47.67%	5.638%
57	8.391	2283	2286	2288	rBV2	1811	1238	0.06%	0.007%
58	8.423	2293	2296	2300	rBV6	1304	1057	0.05%	0.006%
59	8.519	2323	2326	2328	rBV5	1264	768	0.04%	0.004%
60	8.587	2345	2347	2351	rBV5	1787	1485	0.07%	0.008%
61	8.629	2356	2360	2362	rBV3	1054	709	0.03%	0.004%
62	8.857	2417	2431	2459	rBV	1260029	2066975	100.00%	11.826%
63	9.252	2549	2554	2557	rBV5	1244	932	0.05%	0.005%
64	9.326	2573	2577	2581	rBV5	1497	1178	0.06%	0.007%
65	9.349	2581	2584	2588	rVB4	1825	1356	0.07%	0.008%
66	9.371	2588	2591	2594	rBV4	1542	1206	0.06%	0.007%
67	9.465	2617	2620	2630	rVB7	1447	1702	0.08%	0.010%
68	9.593	2657	2660	2664	rBV4	982	749	0.04%	0.004%
69	9.712	2693	2697	2699	rBV3	1707	1329	0.06%	0.008%
70	9.725	2699	2701	2704	rVB4	1439	785	0.04%	0.004%
71	9.747	2704	2708	2710	rBV2	1128	891	0.04%	0.005%
72	9.780	2715	2718	2721	rBV3	2093	1570	0.08%	0.009%
73	10.220	2844	2855	2879	rBV	734623	1122797	54.32%	6.424%
74	10.310	2879	2883	2885	rBV4	1770	1508	0.07%	0.009%
75	10.384	2902	2906	2918	rVB7	6108	9366	0.45%	0.054%
76	10.522	2943	2949	2950	rBV4	1669	1385	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021296.D
 Acq On : 05 May 2021 16:28
 Operator : SY/MD
 Sample : M2271-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

77	10.625	2979	2981	2985	rVB3	1716	882	0.04%	0.005%
78	10.744	3015	3018	3021	rBV5	1046	967	0.05%	0.006%
79	11.001	3095	3098	3100	rBV4	1233	745	0.04%	0.004%
80	11.188	3152	3156	3159	rBV5	1262	1024	0.05%	0.006%
81	11.255	3165	3177	3197	rBV	1336793	2053263	99.34%	11.748%
82	11.554	3267	3270	3271	rBV2	2254	1480	0.07%	0.008%
83	11.632	3281	3294	3312	rBV	1116656	1765977	85.44%	10.104%
84	11.754	3328	3332	3335	rBV5	2819	2758	0.13%	0.016%
85	12.056	3423	3426	3430	rBV3	1154	936	0.05%	0.005%
86	12.255	3483	3488	3492	rBV7	1889	2039	0.10%	0.012%
87	12.506	3559	3566	3569	rBV5	1954	2297	0.11%	0.013%
88	12.683	3619	3621	3624	rVB3	1525	711	0.03%	0.004%
89	12.747	3639	3641	3646	rBV4	879	900	0.04%	0.005%
90	12.863	3675	3677	3680	rBV3	1115	717	0.03%	0.004%
91	12.953	3701	3705	3707	rBV4	1013	792	0.04%	0.005%
92	13.091	3746	3748	3751	rBV2	1476	907	0.04%	0.005%
93	13.381	3836	3838	3841	rBV3	1511	888	0.04%	0.005%
94	13.468	3862	3865	3868	rBV3	1250	967	0.05%	0.006%
95	13.545	3887	3889	3890	rBV	1774	840	0.04%	0.005%
96	13.985	4024	4026	4030	rVB3	1857	1099	0.05%	0.006%
97	14.008	4030	4033	4036	rBV3	1857	1592	0.08%	0.009%
98	14.220	4096	4099	4100	rBV2	1753	956	0.05%	0.005%
99	14.558	4201	4204	4206	rBV3	2048	1451	0.07%	0.008%
100	15.104	4372	4374	4378	rBV3	2434	1661	0.08%	0.010%


Sum of corrected areas: 17477802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021296.D
Acq On : 05 May 2021 16:28
Operator : SY/MD
Sample : M2271-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

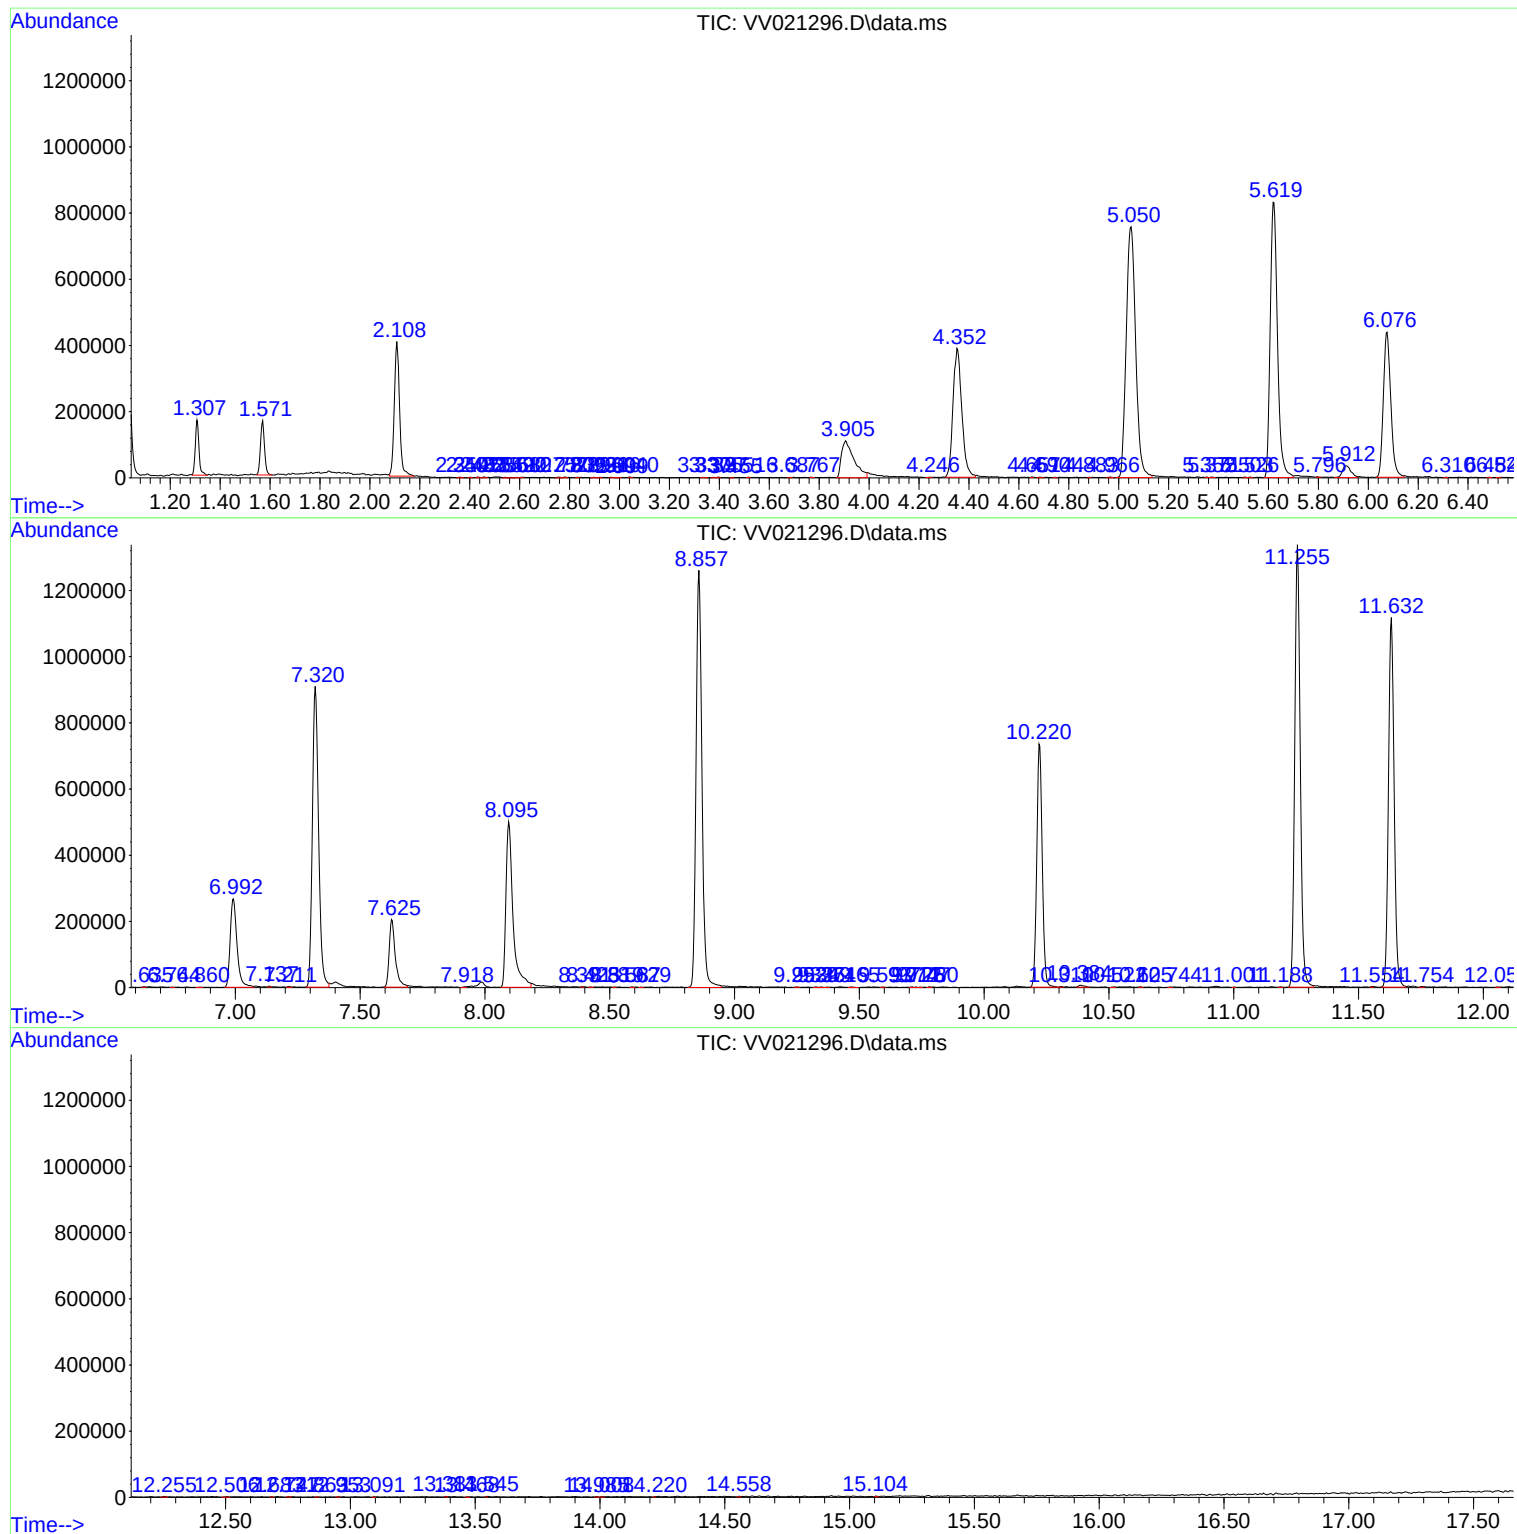

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021296.D
Acq On : 05 May 2021 16:28
Operator : SY/MD
Sample : M2271-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
Data File : VV021296.D
Acq On : 05 May 2021 16:28
Operator : SY/MD
Sample : M2271-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6B5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
