


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050521\
 Data File : VV021279.D
 Acq On : 05 May 2021 08:44
 Operator : SY/MD
 Sample : BFB95
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB195

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis
 Last Update : Thu May 06 02:15:40 2021

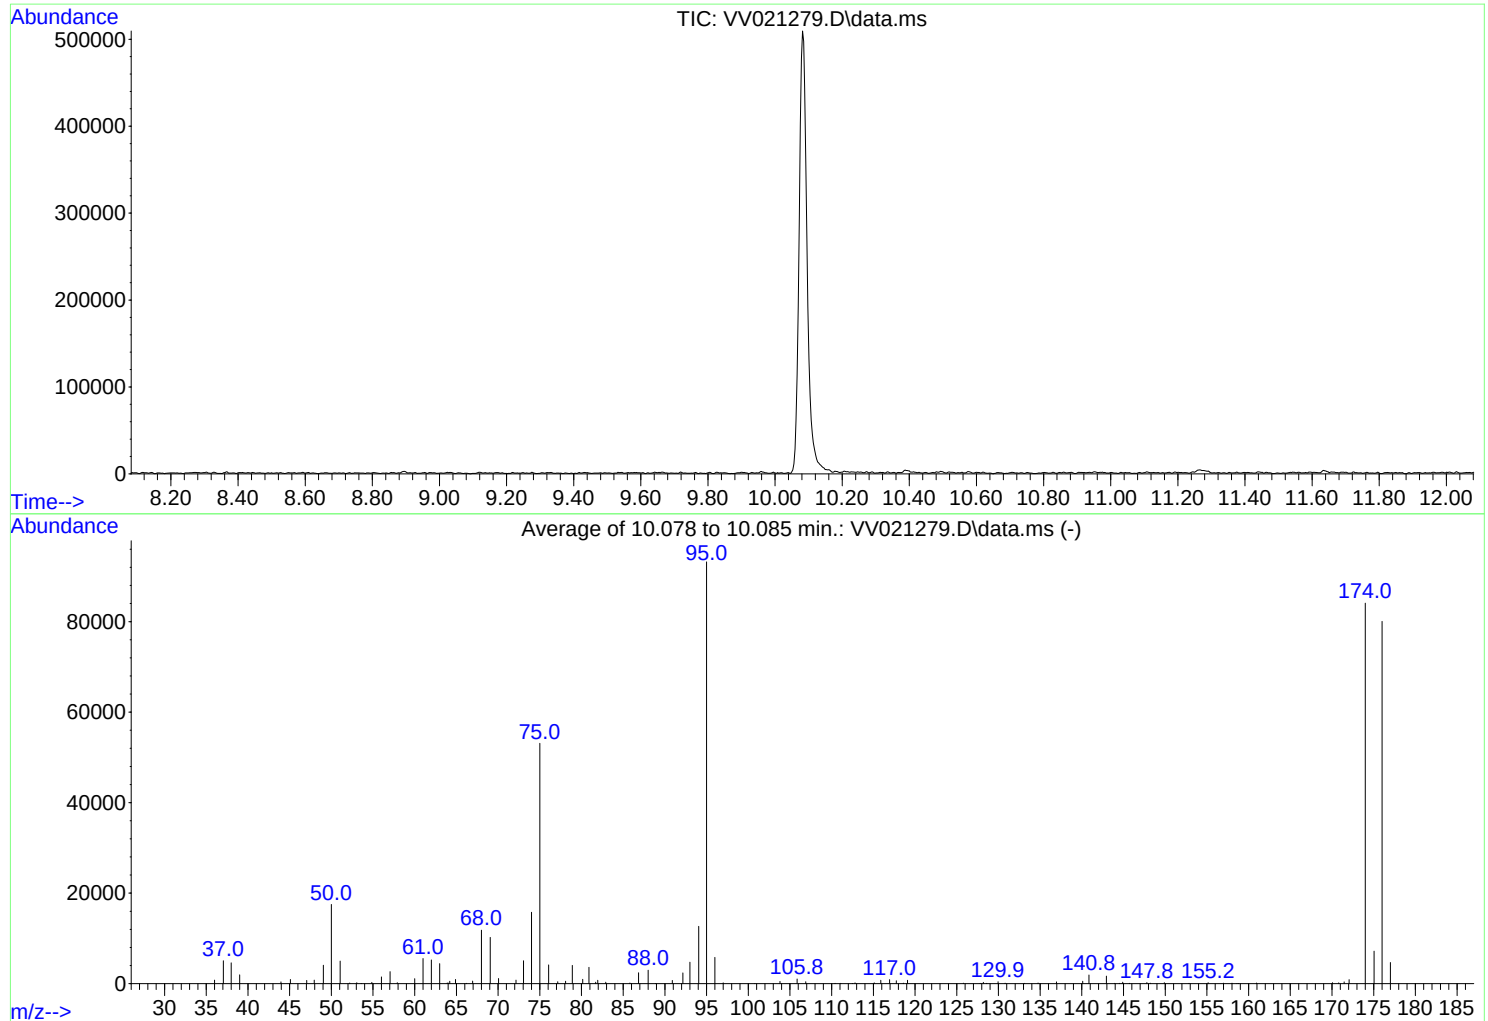

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	17493	PASS
75	95	30	80	57.0	53096	PASS
95	95	100	100	100.0	93216	PASS
96	95	5	9	6.2	5799	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.2	84096	PASS
175	174	5	9	8.5	7176	PASS
176	174	95	105	95.2	80045	PASS
177	176	5	10	5.9	4683	PASS

m/z	Abundance
36.00	600.0
37.00	5294.0
38.00	4336.0
39.00	1919.0
40.00	152.0
43.90	597.0
45.00	975.0
47.10	898.0
47.90	772.0
49.10	4214.0
50.00	17200.0
51.10	5089.0
52.20	166.0
53.10	335.0
54.80	284.0
56.00	1503.0
57.00	2881.0
60.00	879.0
61.00	5439.0
62.00	5324.0
63.00	3940.0
63.90	476.0
64.00	480.0
64.90	830.0
66.20	128.0
67.00	701.0
68.00	11548.0
69.10	9623.0
70.00	896.0
72.20	815.0
73.00	4715.0
74.00	15244.0
75.00	52552.0
76.10	4356.0
77.20	359.0
78.10	483.0
78.90	3533.0
80.10	852.0
80.90	3407.0
81.70	994.0
82.90	129.0
85.80	283.0
86.80	2419.0
88.00	3385.0
90.90	538.0
92.10	2214.0
93.00	5251.0
94.10	11848.0
95.00	91936.0
96.00	5593.0
97.00	195.0
103.80	643.0
105.90	992.0
106.90	294.0
110.40	194.0
111.10	199.0
112.80	220.0
115.10	139.0
115.90	777.0
117.00	1175.0
117.70	530.0
118.60	343.0
119.10	504.0
127.80	193.0
128.30	238.0
130.00	423.0
134.80	160.0
136.90	341.0
140.10	301.0
140.90	2056.0
143.00	1542.0
144.90	400.0
147.70	317.0
148.20	242.0
149.90	120.0
155.20	141.0
157.00	154.0
158.00	184.0
158.60	107.0
160.90	320.0
170.00	190.0
170.80	227.0
171.40	247.0
172.00	928.0
174.00	77856.0
175.00	6714.0
176.00	75392.0
177.00	4425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB195

m/z	Abundance
40.10	174.0
44.10	119.0
78.40	102.0
87.60	125.0
97.70	132.0
167.60	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB195

m/z	Abundance
36.00	989.0
37.10	4677.0
38.00	4769.0
39.00	1951.0
39.90	151.0
44.00	479.0
45.20	813.0
47.00	541.0
48.00	849.0
49.00	3763.0
50.00	17520.0
51.00	4872.0
52.20	128.0
52.90	137.0
53.60	152.0
54.90	288.0
56.00	1343.0
57.10	2370.0
57.90	386.0
60.00	1386.0
61.00	5264.0
62.00	5002.0
63.00	4779.0
64.20	824.0
64.90	991.0
66.80	460.0
68.00	11384.0
69.00	10440.0
70.10	1329.0
72.10	720.0
73.00	5104.0
74.00	16078.0
75.00	53144.0
76.00	3744.0
77.10	498.0
78.10	484.0
78.90	4489.0
80.10	990.0
80.90	3705.0
82.00	1146.0
82.90	507.0
86.90	2285.0
88.00	2371.0
90.90	766.0
92.20	2454.0
93.00	4167.0
94.00	12880.0
95.00	91008.0
96.00	5737.0
97.00	166.0
100.80	110.0
103.80	330.0
105.90	962.0
106.90	473.0
112.50	119.0
112.80	120.0
115.10	204.0
115.90	671.0
116.80	673.0
117.80	683.0
119.10	954.0
125.80	175.0
128.10	304.0
128.60	244.0
129.90	385.0
130.80	203.0
133.10	193.0
134.70	138.0
137.00	375.0
140.10	715.0
140.80	1596.0
143.00	1844.0
144.00	158.0
144.50	199.0
145.00	225.0
145.70	143.0
147.90	246.0
149.90	244.0
152.90	130.0
155.10	288.0
158.80	136.0
170.10	225.0
170.80	136.0
171.50	537.0
172.10	967.0
174.00	87680.0
175.10	7396.0
176.00	82024.0
177.00	4826.0

Instrument :
MSVOA_V
ClientSampleId :
BFB195

m/z	Abundance
36.00	763.0
37.00	5186.0
38.00	4649.0
39.00	1932.0
39.90	121.0
43.90	498.0
45.10	969.0
47.00	691.0
48.00	751.0
49.00	4202.0
50.00	17760.0
51.10	4956.0
52.20	114.0
53.10	216.0
54.80	264.0
56.00	1575.0
57.00	2717.0
57.90	255.0
60.00	1052.0
61.00	5977.0
62.00	5345.0
63.00	4493.0
64.20	739.0
64.90	939.0
66.20	114.0
67.00	555.0
68.00	12527.0
69.00	10576.0
70.10	1163.0
72.20	810.0
73.10	5401.0
74.00	16035.0
75.00	53592.0
76.10	4275.0
77.20	460.0
78.10	601.0
78.90	4091.0
80.20	1022.0
80.90	3712.0
81.90	1086.0
82.90	349.0
85.80	115.0
86.80	2549.0
88.00	3191.0
88.90	109.0
90.90	793.0
92.20	2489.0
93.00	4795.0
94.00	13242.0
95.00	96704.0
96.00	6068.0
97.00	147.0
103.80	517.0
105.80	1149.0
106.90	494.0
112.80	219.0
115.10	169.0
115.90	765.0
117.00	854.0
117.70	662.0
119.10	789.0
125.80	152.0
128.30	268.0
129.90	443.0
130.80	167.0
134.80	148.0
137.00	426.0
140.10	628.0
140.80	2047.0
142.90	1663.0
143.90	105.0
144.90	319.0
145.70	106.0
147.80	225.0
148.20	129.0
149.90	238.0
152.80	139.0
155.20	237.0
157.00	154.0
158.00	116.0
161.00	147.0
170.10	201.0
170.80	201.0
171.50	406.0
172.00	799.0
174.00	86752.0
175.00	7418.0
176.00	82720.0
177.00	4797.0

Instrument :
MSVOA_V
ClientSampleId :
BFB195