

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
 Data File : VV030992.D
 Acq On : 05 May 2023 12:24
 Operator : SY/MD
 Sample : VV0505WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK333

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV	65524	73631	15.25%	1.839%
2	1.536	147	154	167	rVB	61353	73572	15.24%	1.838%
3	2.063	308	318	332	rBV	139507	202102	41.87%	5.049%
4	2.452	430	439	455	rVB6	7672	14375	2.98%	0.359%
5	3.838	859	870	884	rBV2	28293	95684	19.82%	2.390%
6	4.259	986	1001	1022	rBV2	92457	240923	49.91%	6.019%
7	4.966	1204	1221	1243	rBV2	188340	482722	100.00%	12.059%
8	5.542	1387	1400	1422	rBV	155078	330602	68.49%	8.259%
9	5.998	1528	1542	1563	rBV2	113615	244102	50.57%	6.098%
10	6.921	1817	1829	1851	rBV	49415	102351	21.20%	2.557%
11	7.252	1920	1932	1955	rBV	203621	369058	76.45%	9.220%
12	7.564	2016	2029	2046	rBV2	29789	62322	12.91%	1.557%
13	8.037	2166	2176	2215	rBV	163265	406453	84.20%	10.154%
14	8.793	2400	2411	2428	rBV	241129	403664	83.62%	10.084%
15	10.162	2825	2837	2847	rBV	86389	141862	29.39%	3.544%
16	11.194	3146	3158	3174	rBV	237815	386314	80.03%	9.651%
17	11.567	3263	3274	3290	rBV	219281	354913	73.52%	8.866%
18	12.201	3463	3471	3478	rBV10	4002	5717	1.18%	0.143%
19	13.455	3853	3861	3871	rBV7	4699	6923	1.43%	0.173%
20	13.693	3928	3935	3943	rBV10	3878	5703	1.18%	0.142%




Sum of corrected areas: 4002993

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
Data File : VV030992.D
Acq On : 05 May 2023 12:24
Operator : SY/MD
Sample : VV0505WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

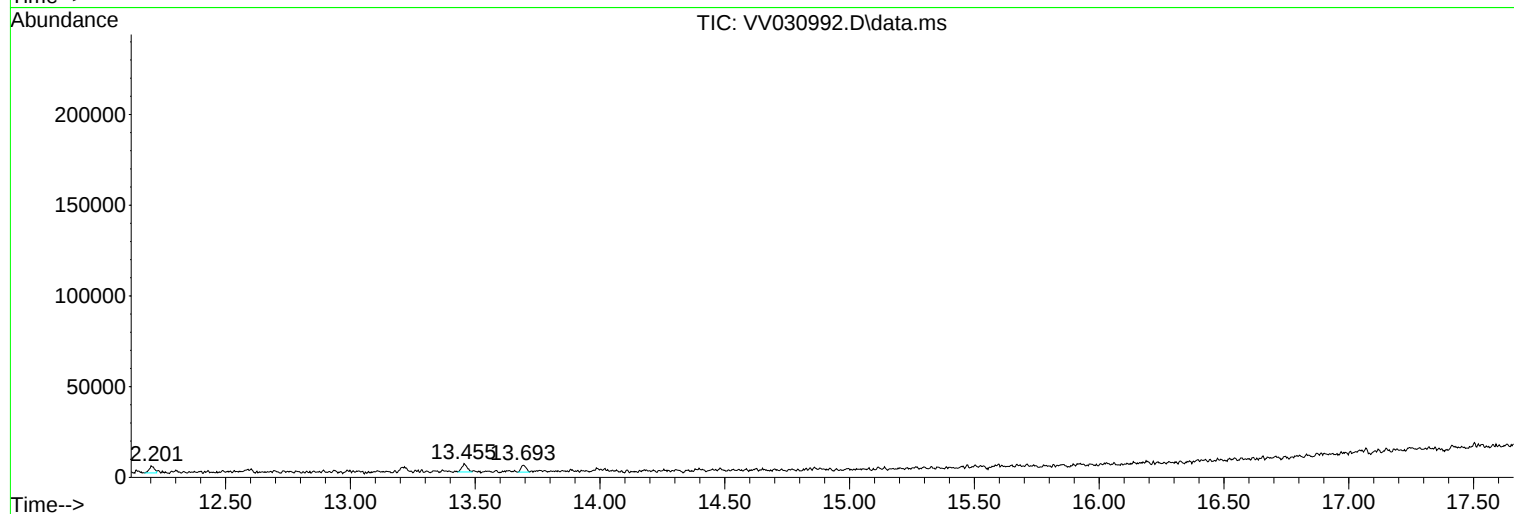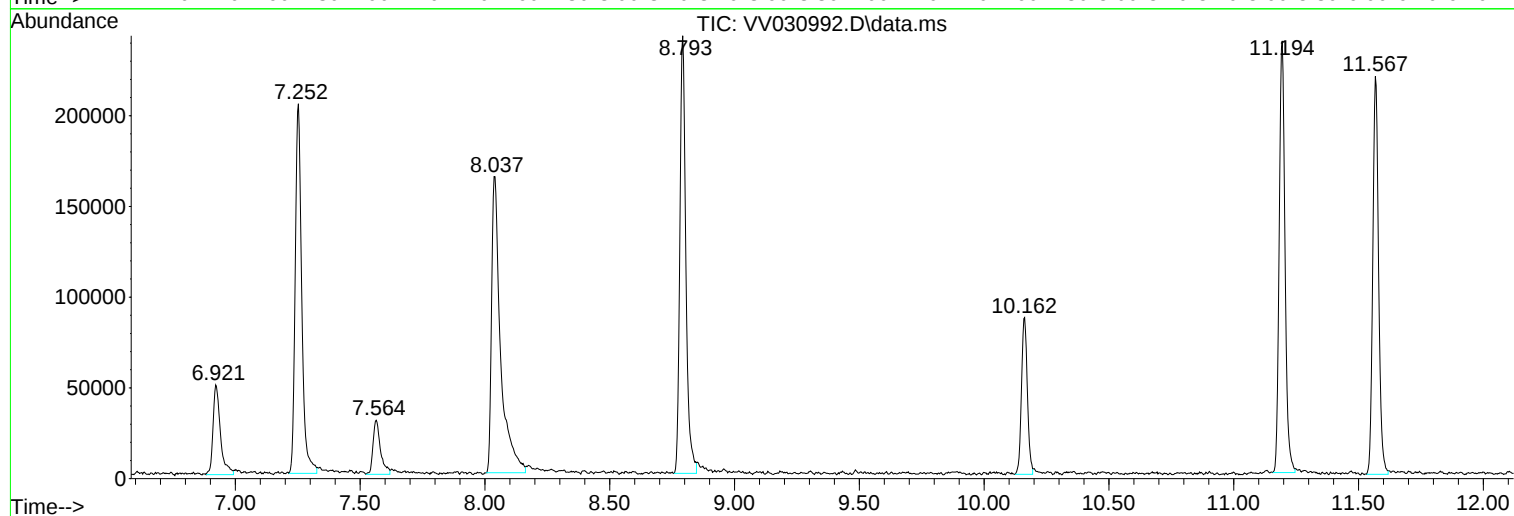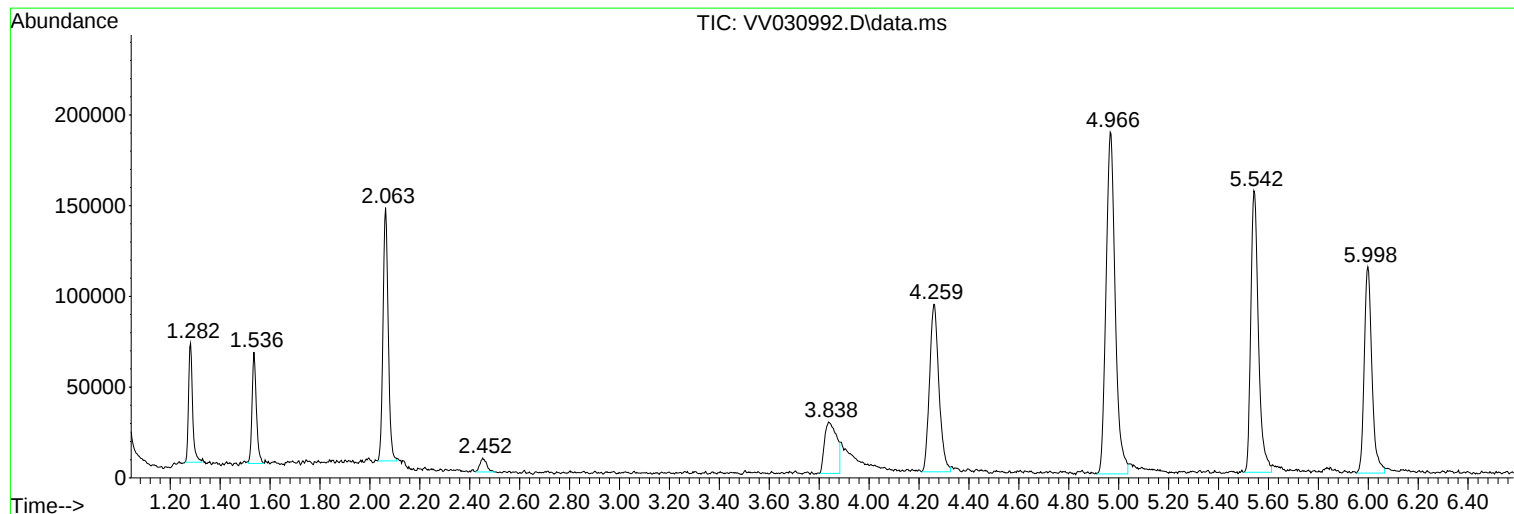

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
Data File : VV030992.D
Acq On : 05 May 2023 12:24
Operator : SY/MD
Sample : VV0505WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
Data File : VV030992.D
Acq On : 05 May 2023 12:24
Operator : SY/MD
Sample : VV0505WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK333

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc