

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
 Data File : VV030998.D
 Acq On : 05 May 2023 16:43
 Operator : SY/MD
 Sample : 02613-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rVB	61444	69866	15.64%	2.240%
2	1.535	147	154	166	rBV	58402	72947	16.33%	2.339%
3	2.063	309	318	329	rVV	129332	188450	42.20%	6.043%
4	2.117	332	335	345	rVB	7952	9179	2.06%	0.294%
5	2.455	428	440	451	rVB3	9538	16868	3.78%	0.541%
6	3.850	858	874	888	rBV2	23871	92548	20.72%	2.968%
7	4.262	985	1002	1025	rBV	88065	232642	52.09%	7.460%
8	4.966	1205	1221	1250	rBV2	167714	446597	100.00%	14.322%
9	5.545	1387	1401	1419	rBV	124174	266400	59.65%	8.543%
10	5.998	1527	1542	1562	rBV2	107866	233158	52.21%	7.477%
11	6.924	1820	1830	1848	rBV	45907	90345	20.23%	2.897%
12	7.252	1921	1932	1957	rBV	149488	275105	61.60%	8.822%
13	7.564	2020	2029	2042	rBV2	27062	53713	12.03%	1.722%
14	7.886	2120	2129	2135	rBV7	3404	4836	1.08%	0.155%
15	8.040	2165	2177	2215	rBV	151221	407128	91.16%	13.056%
16	8.792	2400	2411	2430	rBV	151784	265990	59.56%	8.530%
17	10.162	2825	2837	2854	rBV	81340	137005	30.68%	4.394%
18	10.332	2880	2890	2900	rVB2	8869	14651	3.28%	0.470%
19	11.194	3149	3158	3175	rBV	74557	123486	27.65%	3.960%
20	11.570	3263	3275	3290	rBV	69999	117422	26.29%	3.766%




Sum of corrected areas: 3118336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
Data File : VV030998.D
Acq On : 05 May 2023 16:43
Operator : SY/MD
Sample : 02613-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

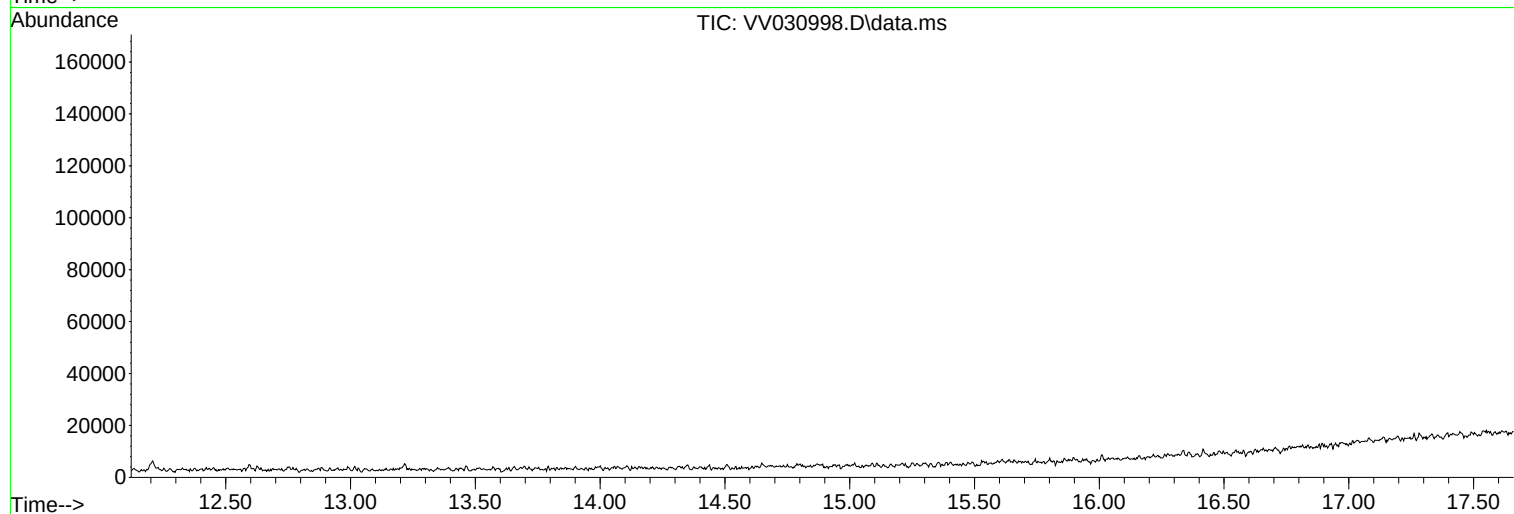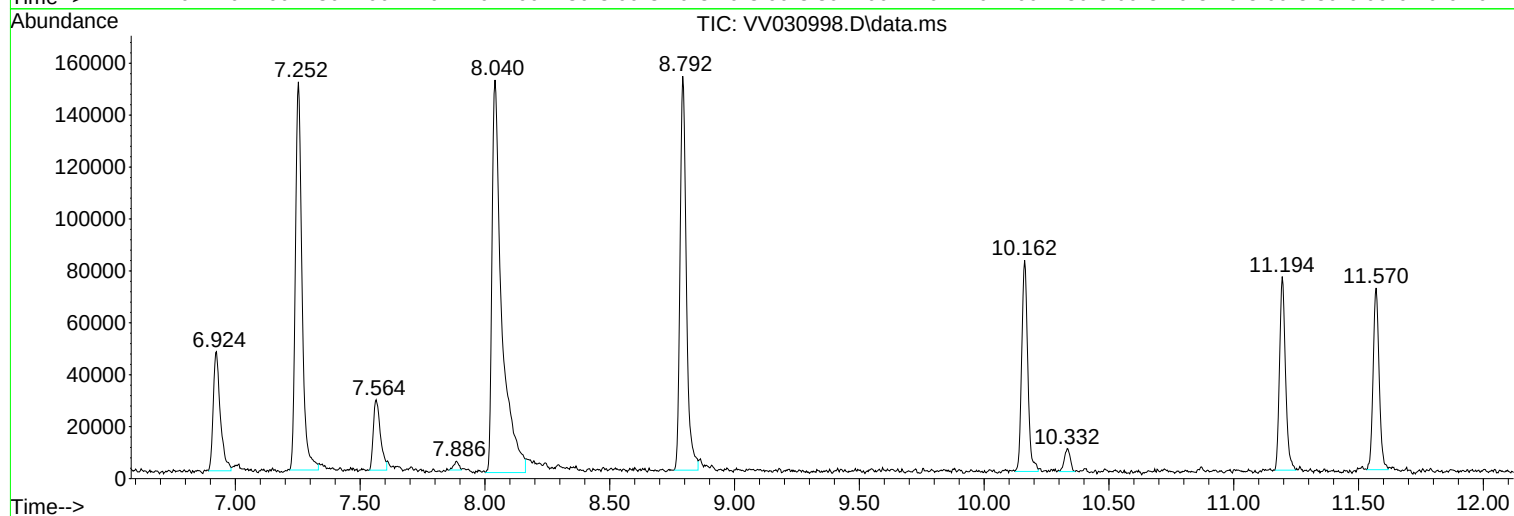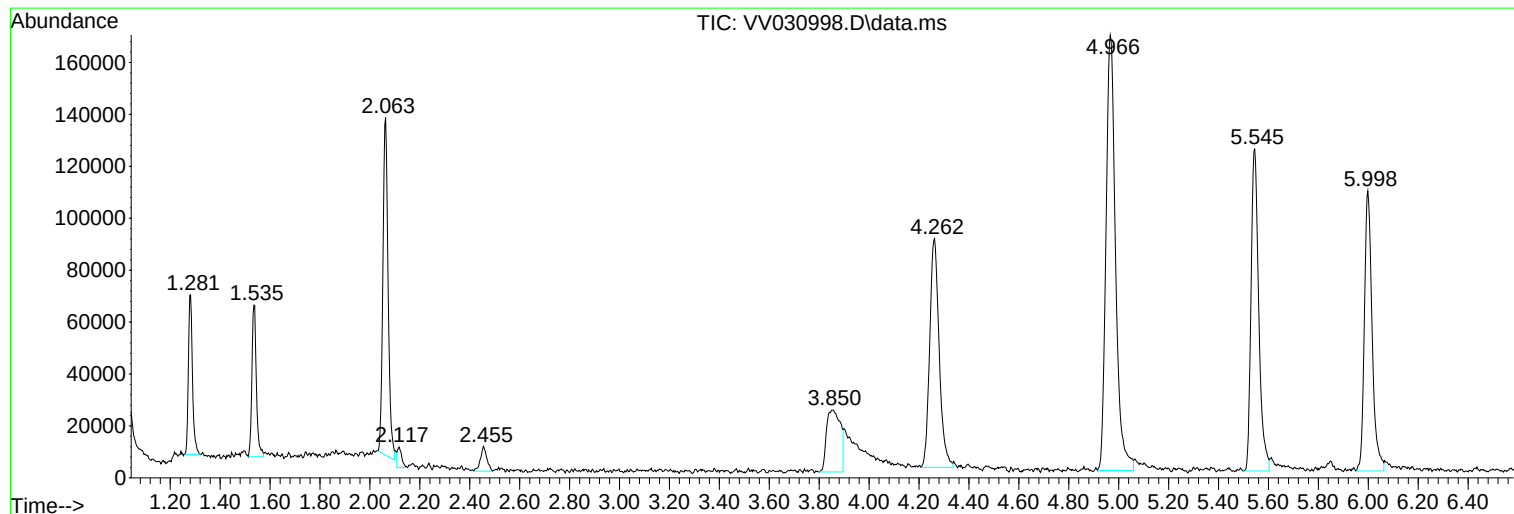

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
Data File : VV030998.D
Acq On : 05 May 2023 16:43
Operator : SY/MD
Sample : 02613-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
Data File : VV030998.D
Acq On : 05 May 2023 16:43
Operator : SY/MD
Sample : 02613-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc