
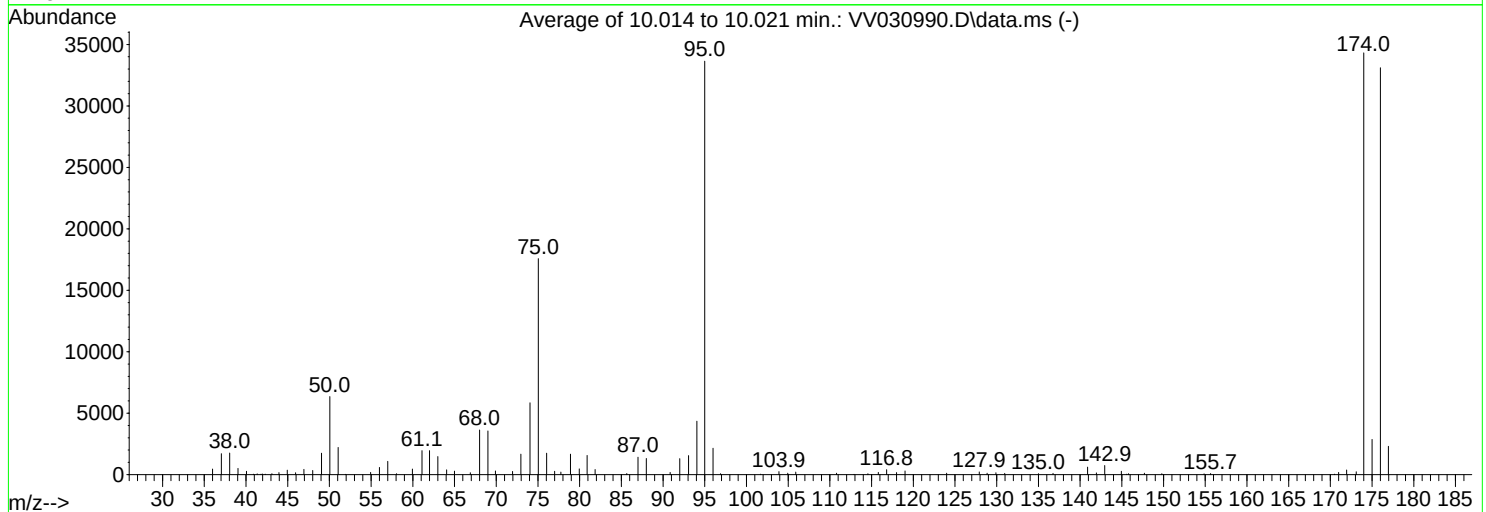


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050523\
 Data File : VV030990.D
 Acq On : 05 May 2023 11:08
 Operator : SY/MD
 Sample : BFB258
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB258

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat May 06 01:44:36 2023

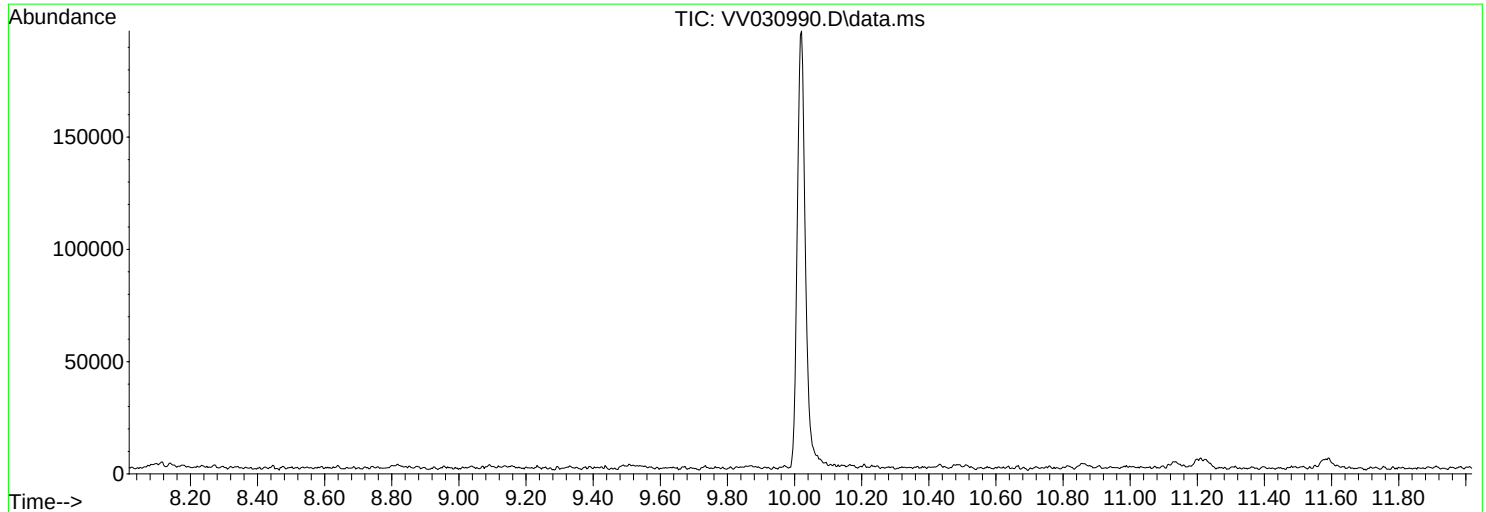

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	6353	PASS
75	95	30	80	52.2	17573	PASS
95	95	100	100	100.0	33637	PASS
96	95	5	9	6.4	2146	PASS
173	174	0.00	2	0.7	232	PASS
174	95	50	120	102.0	34320	PASS
175	174	5	9	8.3	2860	PASS
176	174	95	105	96.5	33112	PASS
177	176	5	10	7.0	2306	PASS

m/z	Abundance
36.60	120.0
37.50	132.0
38.60	173.0
39.10	127.0
39.80	233.0
40.60	129.0
43.90	303.0
45.00	112.0
46.70	117.0
48.60	102.0
51.90	160.0
53.10	108.0
55.70	108.0
56.50	137.0
58.50	165.0
59.70	153.0
61.50	117.0
72.90	133.0
85.30	115.0
99.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
36.00	440.0
37.00	1702.0
38.10	1635.0
39.10	673.0
40.20	221.0
41.30	101.0
44.00	453.0
45.00	436.0
45.90	157.0
46.90	424.0
48.00	276.0
49.00	1590.0
50.00	6323.0
51.00	2076.0
52.00	154.0
55.00	202.0
56.00	518.0
57.00	1062.0
58.10	128.0
58.70	103.0
60.00	445.0
61.10	1890.0
62.00	1938.0
63.00	1342.0
64.10	400.0
65.00	253.0
66.90	135.0
68.00	3238.0
69.00	3258.0
69.90	317.0
71.90	228.0
73.00	1576.0
74.00	5507.0
75.10	16384.0
76.10	1716.0
77.10	250.0
77.80	201.0
78.90	1602.0
79.90	461.0
80.90	1555.0
81.80	371.0
87.00	1381.0
88.00	1198.0
91.00	166.0
92.00	1216.0
93.10	1470.0
94.00	4191.0
95.00	31960.0
96.00	1903.0
96.90	127.0
101.70	101.0
103.80	240.0
104.90	107.0
105.90	208.0
110.90	104.0
112.90	100.0
115.80	142.0
116.80	374.0
118.10	166.0
119.00	347.0
124.00	108.0
127.90	199.0
128.80	128.0
129.80	165.0
131.00	113.0
136.70	106.0
140.90	559.0
141.90	153.0
143.00	699.0
145.00	297.0
145.60	105.0
147.70	112.0
149.80	126.0
155.70	130.0
170.50	128.0
171.00	158.0
171.90	328.0
173.10	696.0
174.00	30432.0
175.00	2661.0
176.00	30704.0
176.90	2148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
36.00	491.0
37.00	1738.0
38.00	1803.0
39.00	610.0
40.00	263.0
41.40	111.0
41.80	117.0
42.30	114.0
43.10	109.0
44.00	454.0
45.00	474.0
45.90	156.0
47.00	453.0
48.00	351.0
49.10	1795.0
50.10	6511.0
51.10	2297.0
52.10	194.0
54.90	195.0
56.00	607.0
57.00	1085.0
58.00	104.0
59.90	446.0
61.10	1964.0
62.00	2037.0
63.00	1511.0
64.00	402.0
65.00	273.0
66.90	169.0
68.00	3745.0
69.00	3724.0
69.90	318.0
72.00	268.0
73.00	1918.0
74.00	5977.0
75.00	18072.0
76.00	1769.0
77.00	257.0
77.70	216.0
78.90	1691.0
79.90	470.0
80.90	1596.0
81.90	422.0
85.70	128.0
87.00	1452.0
88.00	1328.0
90.80	172.0
92.00	1371.0
93.10	1592.0
94.00	4453.0
95.00	34760.0
96.00	2200.0
96.90	110.0
103.90	244.0
104.90	136.0
105.90	208.0
110.80	128.0
114.60	115.0
115.80	183.0
116.80	424.0
118.10	159.0
119.00	299.0
124.00	147.0
127.90	243.0
128.90	118.0
129.90	139.0
131.00	114.0
135.00	108.0
136.80	103.0
140.90	654.0
142.00	157.0
143.00	766.0
144.90	281.0
145.80	110.0
147.70	129.0
149.80	129.0
154.90	108.0
155.60	128.0
171.00	196.0
171.90	399.0
174.00	35272.0
175.00	2964.0
176.00	34024.0
176.90	2378.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258

m/z	Abundance
36.00	440.0
37.10	1670.0
38.00	1837.0
39.00	619.0
40.00	327.0
40.90	113.0
42.00	177.0
43.10	144.0
44.00	512.0
44.90	521.0
46.00	153.0
47.00	410.0
48.00	382.0
49.10	1844.0
50.00	6226.0
51.00	2275.0
52.10	212.0
54.90	168.0
56.00	626.0
57.00	1102.0
59.90	467.0
61.10	1991.0
62.00	1877.0
63.00	1563.0
64.00	390.0
65.00	321.0
66.90	174.0
68.00	3903.0
69.00	3700.0
69.90	279.0
72.00	273.0
73.00	1909.0
74.10	6071.0
75.00	18264.0
76.00	1741.0
76.90	299.0
77.80	229.0
78.90	1722.0
80.00	468.0
80.90	1547.0
81.90	448.0
85.60	129.0
87.00	1409.0
88.00	1403.0
90.80	216.0
92.00	1340.0
93.00	1601.0
94.10	4413.0
95.00	34192.0
96.00	2334.0
104.00	247.0
105.00	126.0
105.90	212.0
110.70	108.0
114.50	136.0
115.80	218.0
116.80	417.0
117.90	196.0
119.00	246.0
124.00	110.0
127.90	211.0
128.90	126.0
130.00	153.0
130.80	106.0
135.00	131.0
136.80	111.0
140.90	630.0
142.00	123.0
142.90	765.0
144.90	266.0
145.80	120.0
147.70	128.0
154.80	112.0
171.00	200.0
172.00	427.0
174.00	37256.0
175.00	2956.0
176.00	34608.0
177.00	2392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB258