
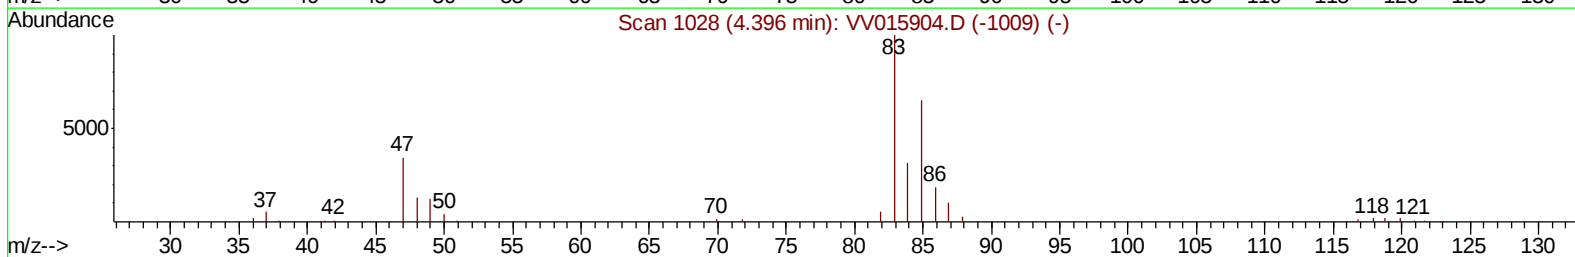
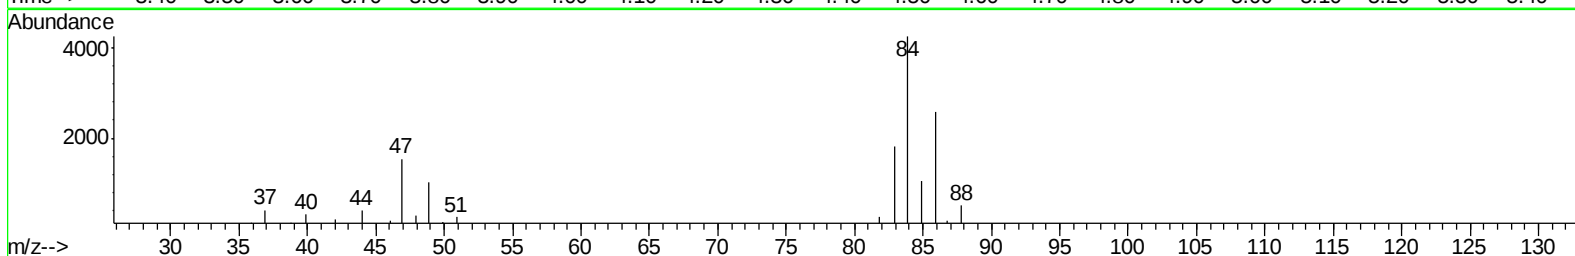


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050620\
Data File : VV015905.D
Acq On : 06 May 2020 13:10
Operator : SY/MD
Sample : VV0506WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: May 07 02:03:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050520WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 07 02:01:25 2020
Response via : Initial Calibration

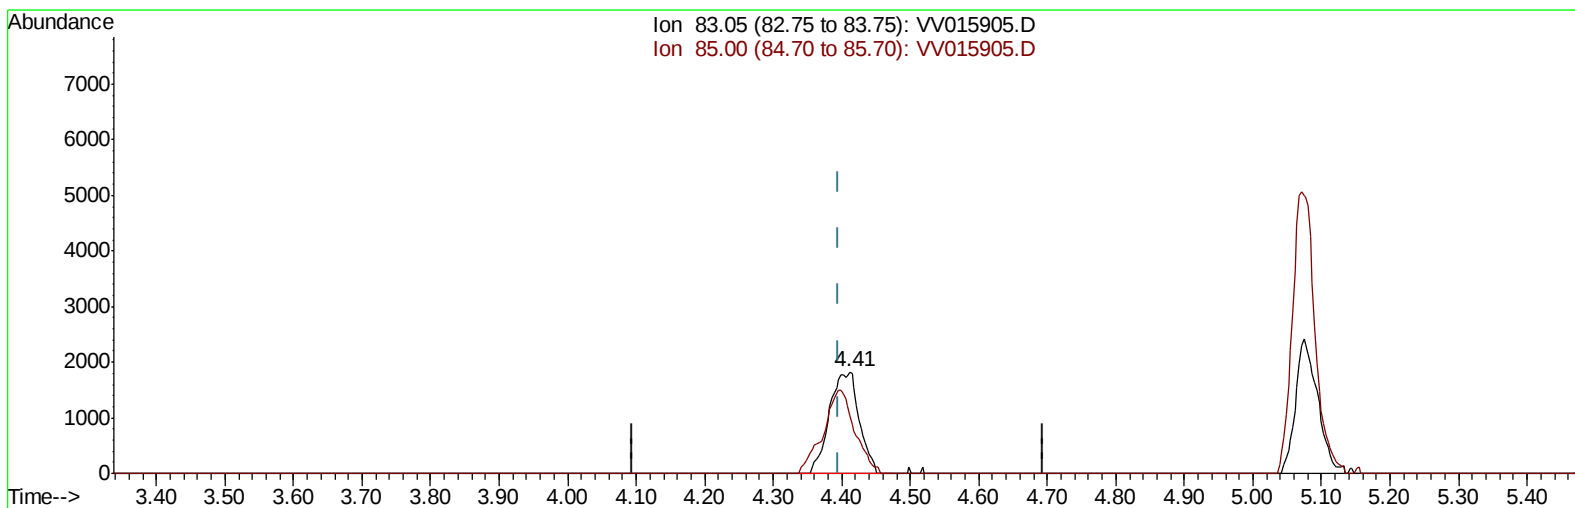

TIC: VV015905.D

(25) Chloroform (T)

4.412min (+0.016) 0.27ug/L m

response 5464

Ion	Exp%	Act%
83.05	100	100
85.00	65.30	57.42
0.00	0.00	0.00
0.00	0.00	0.00