
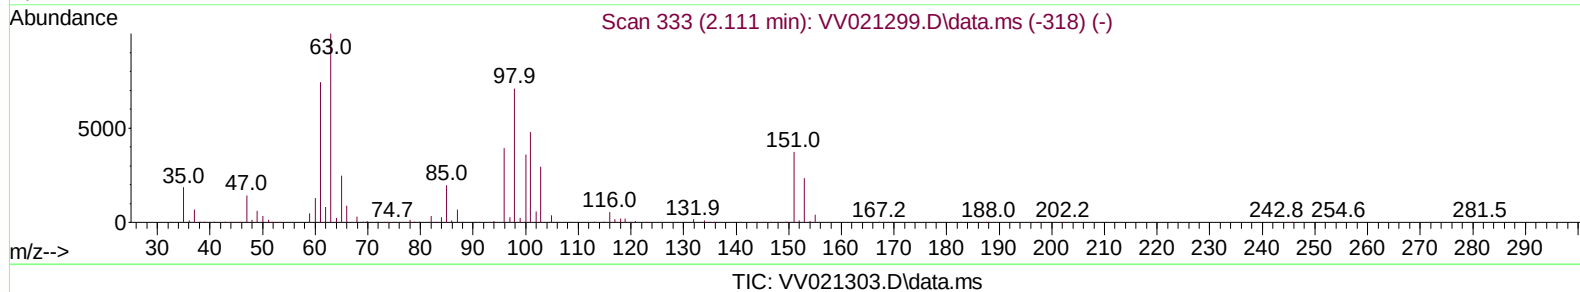
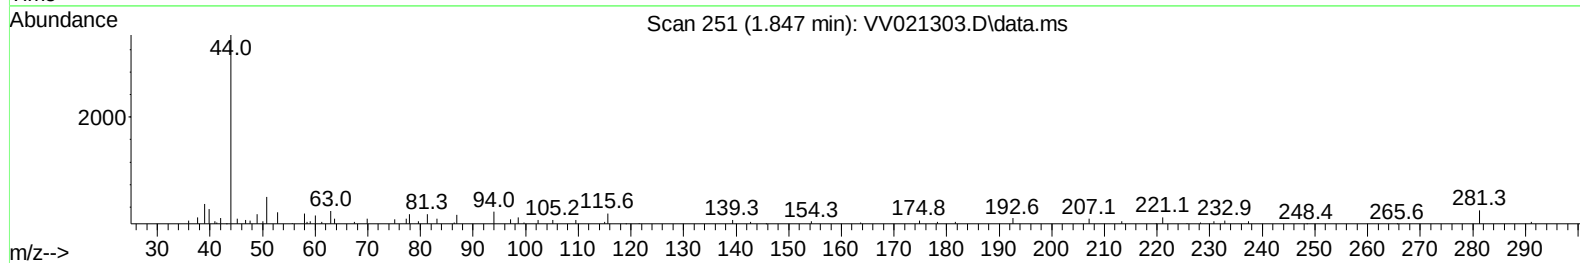


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050621\
Data File : VV021303.D
Acq On : 06 May 2021 12:44
Operator : SY/MD
Sample : M2271-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 07 03:57:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 07 03:56:18 2021
Response via : Initial Calibration

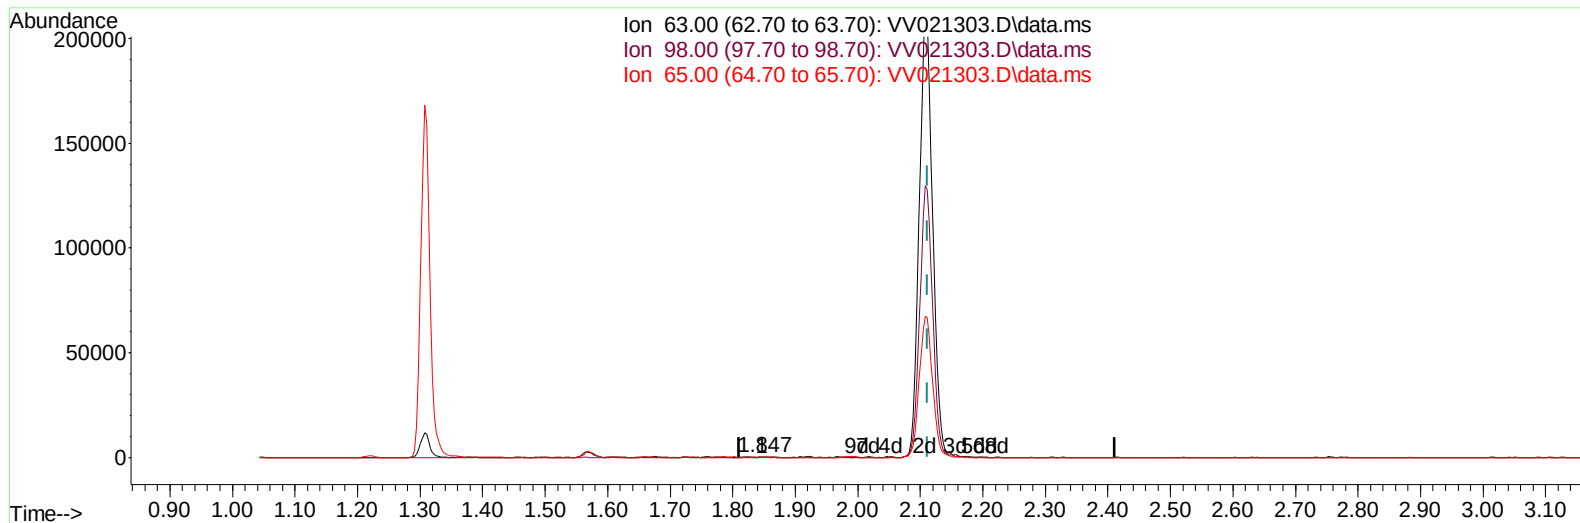

(11) 1,1-Dichloroethene-d2 (S)

1.847min (-0.264) 0.03 ug/L

response 254

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.70	52.36
65.00	23.70	29.92
0.00	0.00	0.00