
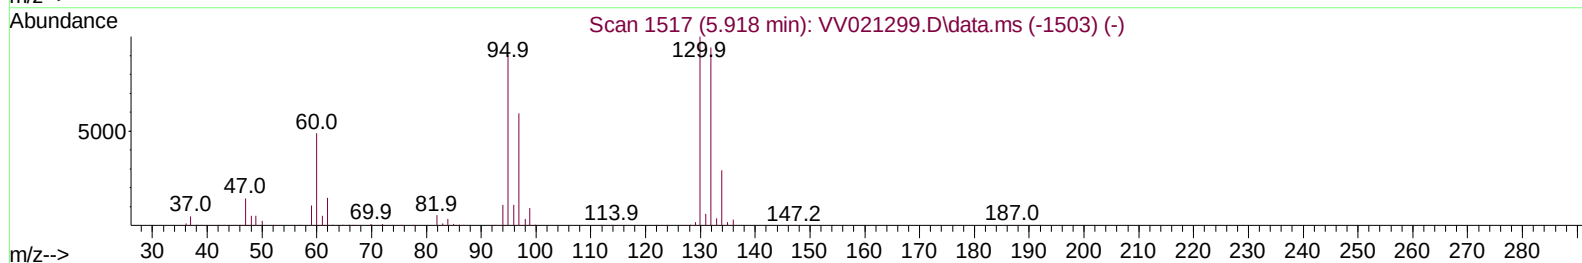
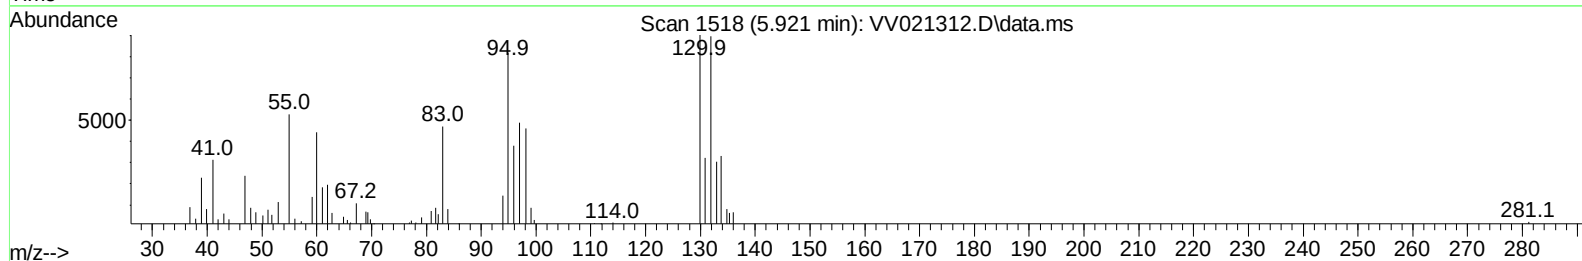


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050621\
Data File : VV021312.D
Acq On : 06 May 2021 17:13
Operator : SY/MD
Sample : M2320-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: May 07 03:58:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 07 03:56:18 2021
Response via : Initial Calibration

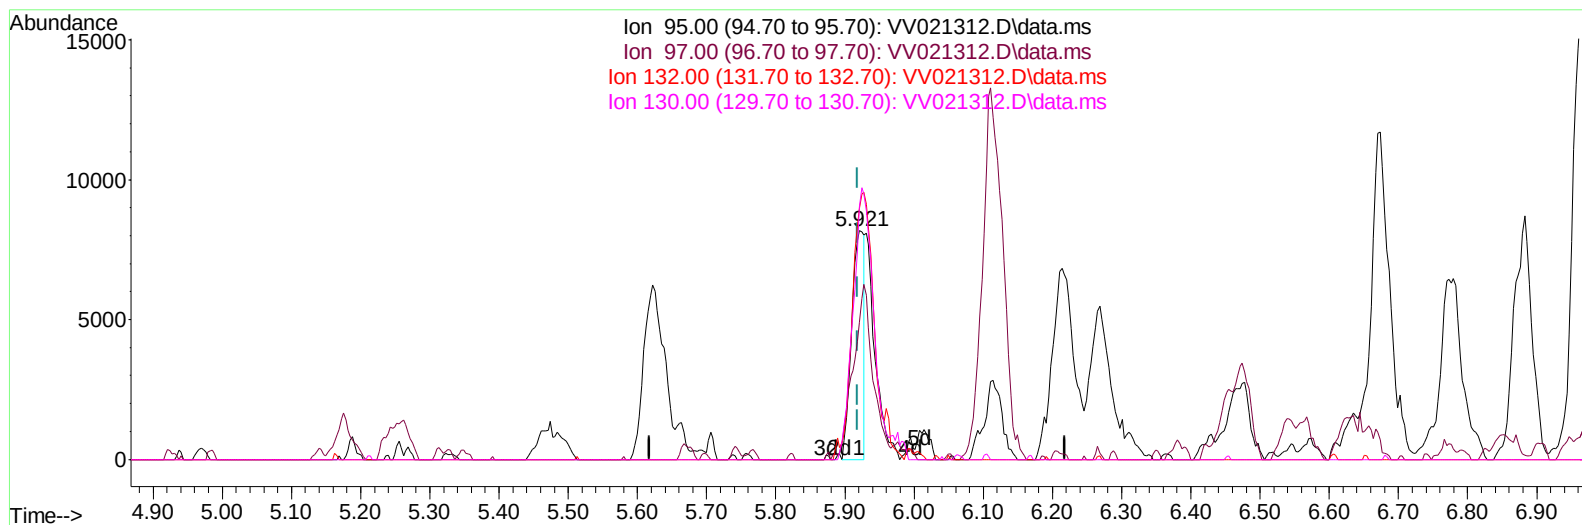

TIC: VV021312.D\data.ms

(34) Trichloroethene (T)**5.921min (+ 0.003) 3.12 ug/L****response 10388**

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	65.00	59.84
132.00	101.40	109.73
130.00	108.20	110.47