

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050621\
 Data File : VV021300.D
 Acq On : 06 May 2021 11:34
 Operator : SY/MD
 Sample : VV0506MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 07 03:56:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 07 03:56:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	673237	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	643119	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	340930	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	167175	55.98	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	111.96%		
7) Chloroethane-d5	1.571	69	143491	53.77	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	107.54%		
11) 1,1-Dichloroethene-d2	2.108	63	311967	37.45	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.90%		
21) 2-Butanone-d5	3.902	46	160056	66.79	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	66.79%		
24) Chloroform-d	4.346	84	443037	46.61	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.22%		
26) 1,2-Dichloroethane-d4	5.031	65	349885	49.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.34%		
32) Benzene-d6	5.050	84	765541	51.69	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.38%		
36) 1,2-Dichloropropane-d6	6.297	67	189	0.05	ug/L	0.23
Spiked Amount 50.000	Range 70 - 120		Recovery =	0.10%#		
41) Toluene-d8	7.317	98	765859	49.90	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.80%		
43) trans-1,3-Dichloroprop...	7.622	79	137775	48.69	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.38%		
47) 2-Hexanone-d5	8.092	63	133988	76.26	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	76.26%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	254668	41.83	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.66%		
66) 1,2-Dichlorobenzene-d4	11.632	152	328448	48.89	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.78%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.629	75	7194	0.97	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050621\
Data File : VV021300.D
Acq On : 06 May 2021 11:34
Operator : SY/MD
Sample : VV0506MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 07 03:56:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 07 03:56:18 2021
Response via : Initial Calibration

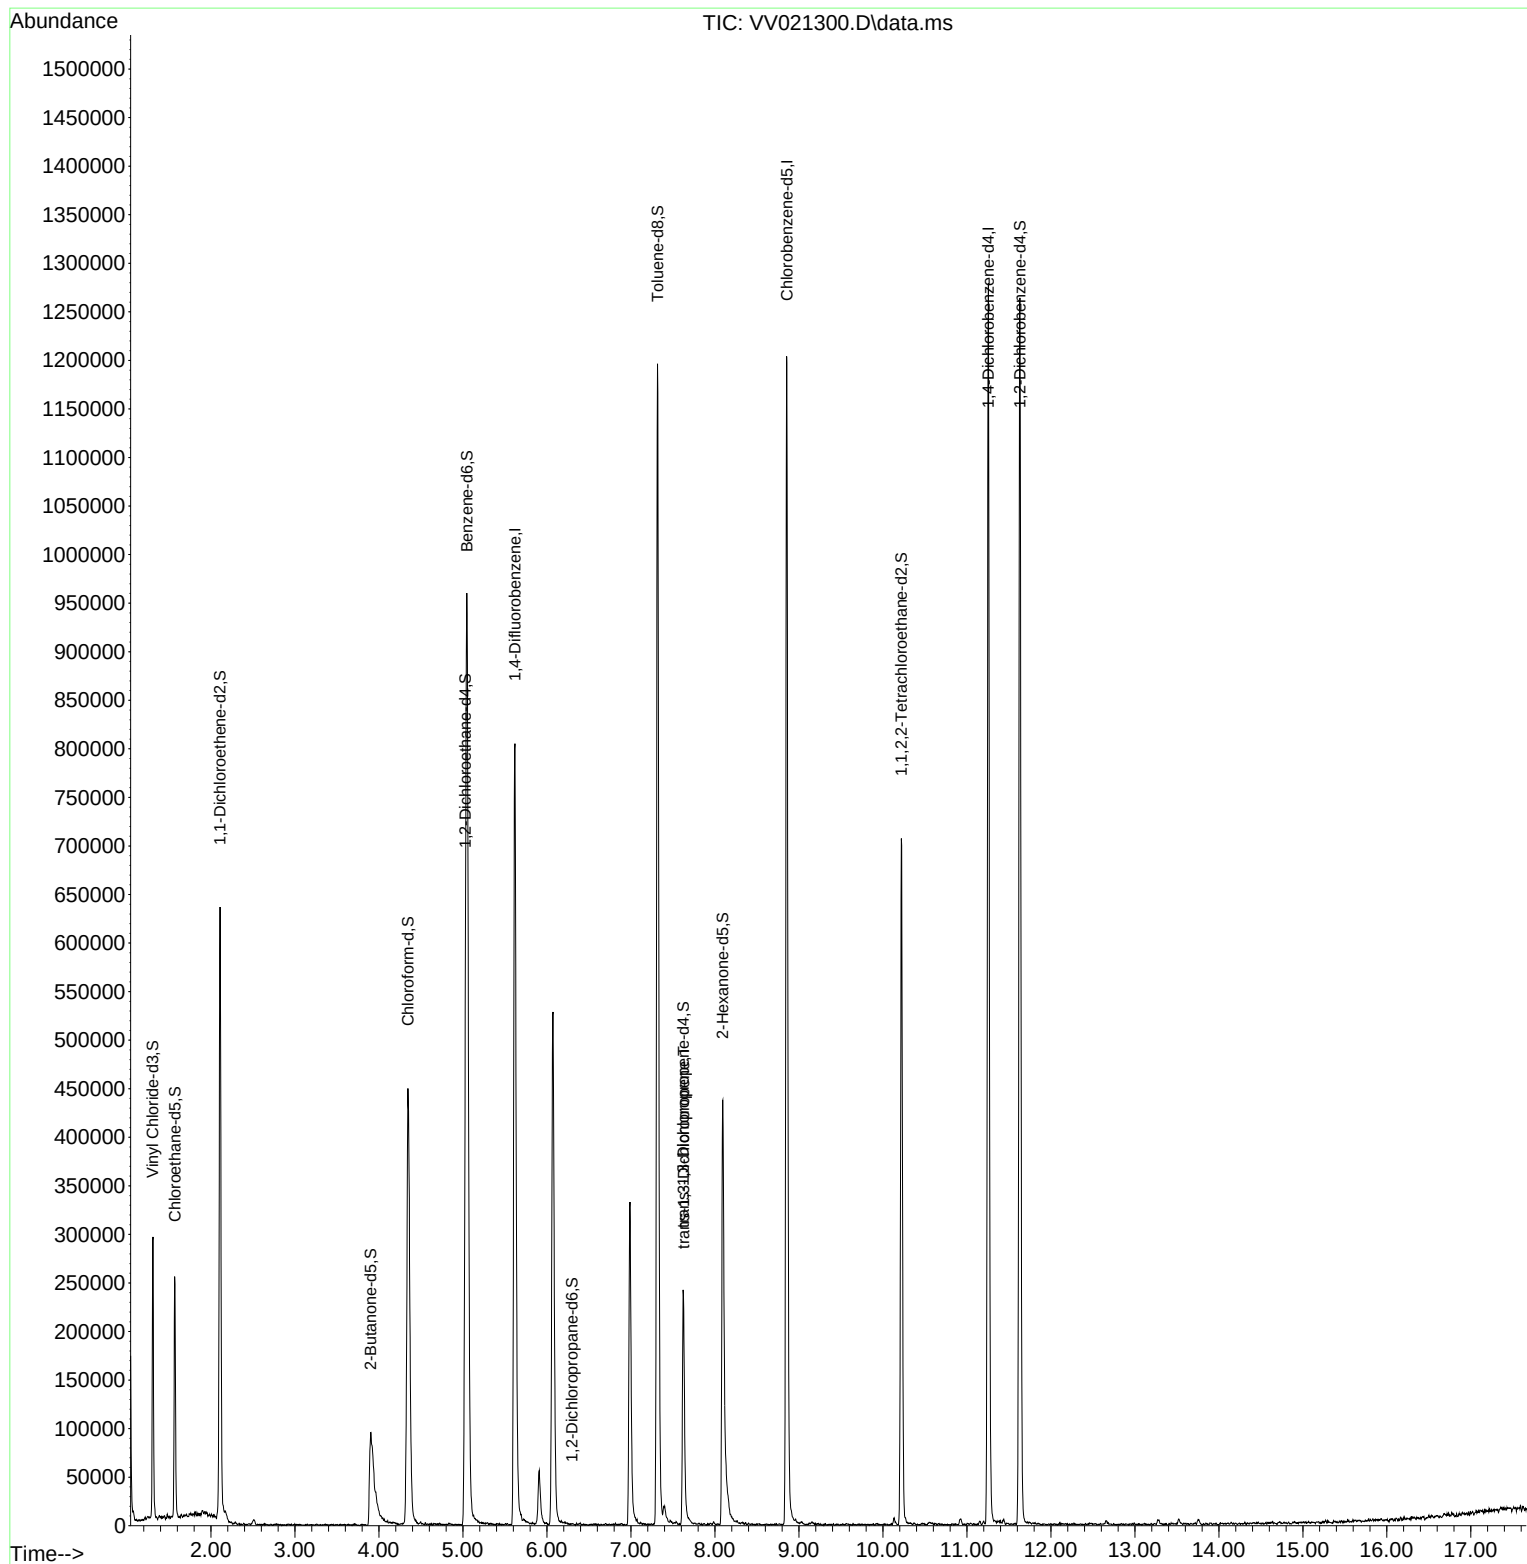

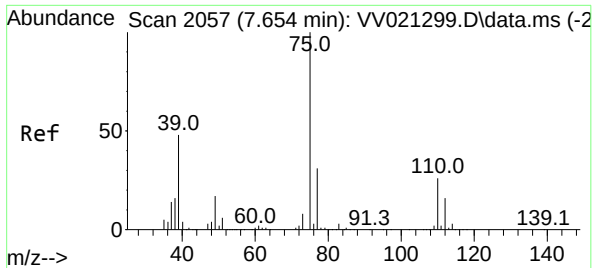

#44
 trans-1,3-Dichloropropene
 Concen: 0.97 ug/L
 RT: 7.629 min Scan# 2049
 Delta R.T. -0.026 min
 Lab File: VV021300.D
 Acq: 06 May 2021 11:34

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 7194
 Ion Ratio Lower Upper
 75 100
 77 36.6 21.8 40.6

