

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050621\
 Data File : VV021309.D
 Acq On : 06 May 2021 15:08
 Operator : SY/MD
 Sample : M2271-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: May 07 03:57:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 07 03:56:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	671616	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	651086	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	328428	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	165110	55.42	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	110.84%	
7) Chloroethane-d5	1.571	69	137978	51.82	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	103.64%	
11) 1,1-Dichloroethene-d2	2.108	63	301183	36.24	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	72.48%	
21) 2-Butanone-d5	3.908	46	220767	92.35	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	92.35%	
24) Chloroform-d	4.352	84	429554	45.30	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.60%	
26) 1,2-Dichloroethane-d4	5.037	65	331525	46.71	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.42%	
32) Benzene-d6	5.056	84	730202	48.70	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.40%	
36) 1,2-Dichloropropane-d6	6.076	67	180873	46.96	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	93.92%	
41) Toluene-d8	7.320	98	721479	46.43	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.86%	
43) trans-1,3-Dichloroprop...	7.625	79	126667	44.21	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.42%	
47) 2-Hexanone-d5	8.095	63	150131	84.40	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	84.40%	
56) 1,1,2,2-Tetrachloroeth...	10.223	84	262793	42.64	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	85.28%	
66) 1,2-Dichlorobenzene-d4	11.632	152	320028	49.45	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.90%	
Target Compounds						
16) Methylene chloride	2.513	84	5988	1.39	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050621\
Data File : VV021309.D
Acq On : 06 May 2021 15:08
Operator : SY/MD
Sample : M2271-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: May 07 03:57:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 07 03:56:18 2021
Response via : Initial Calibration

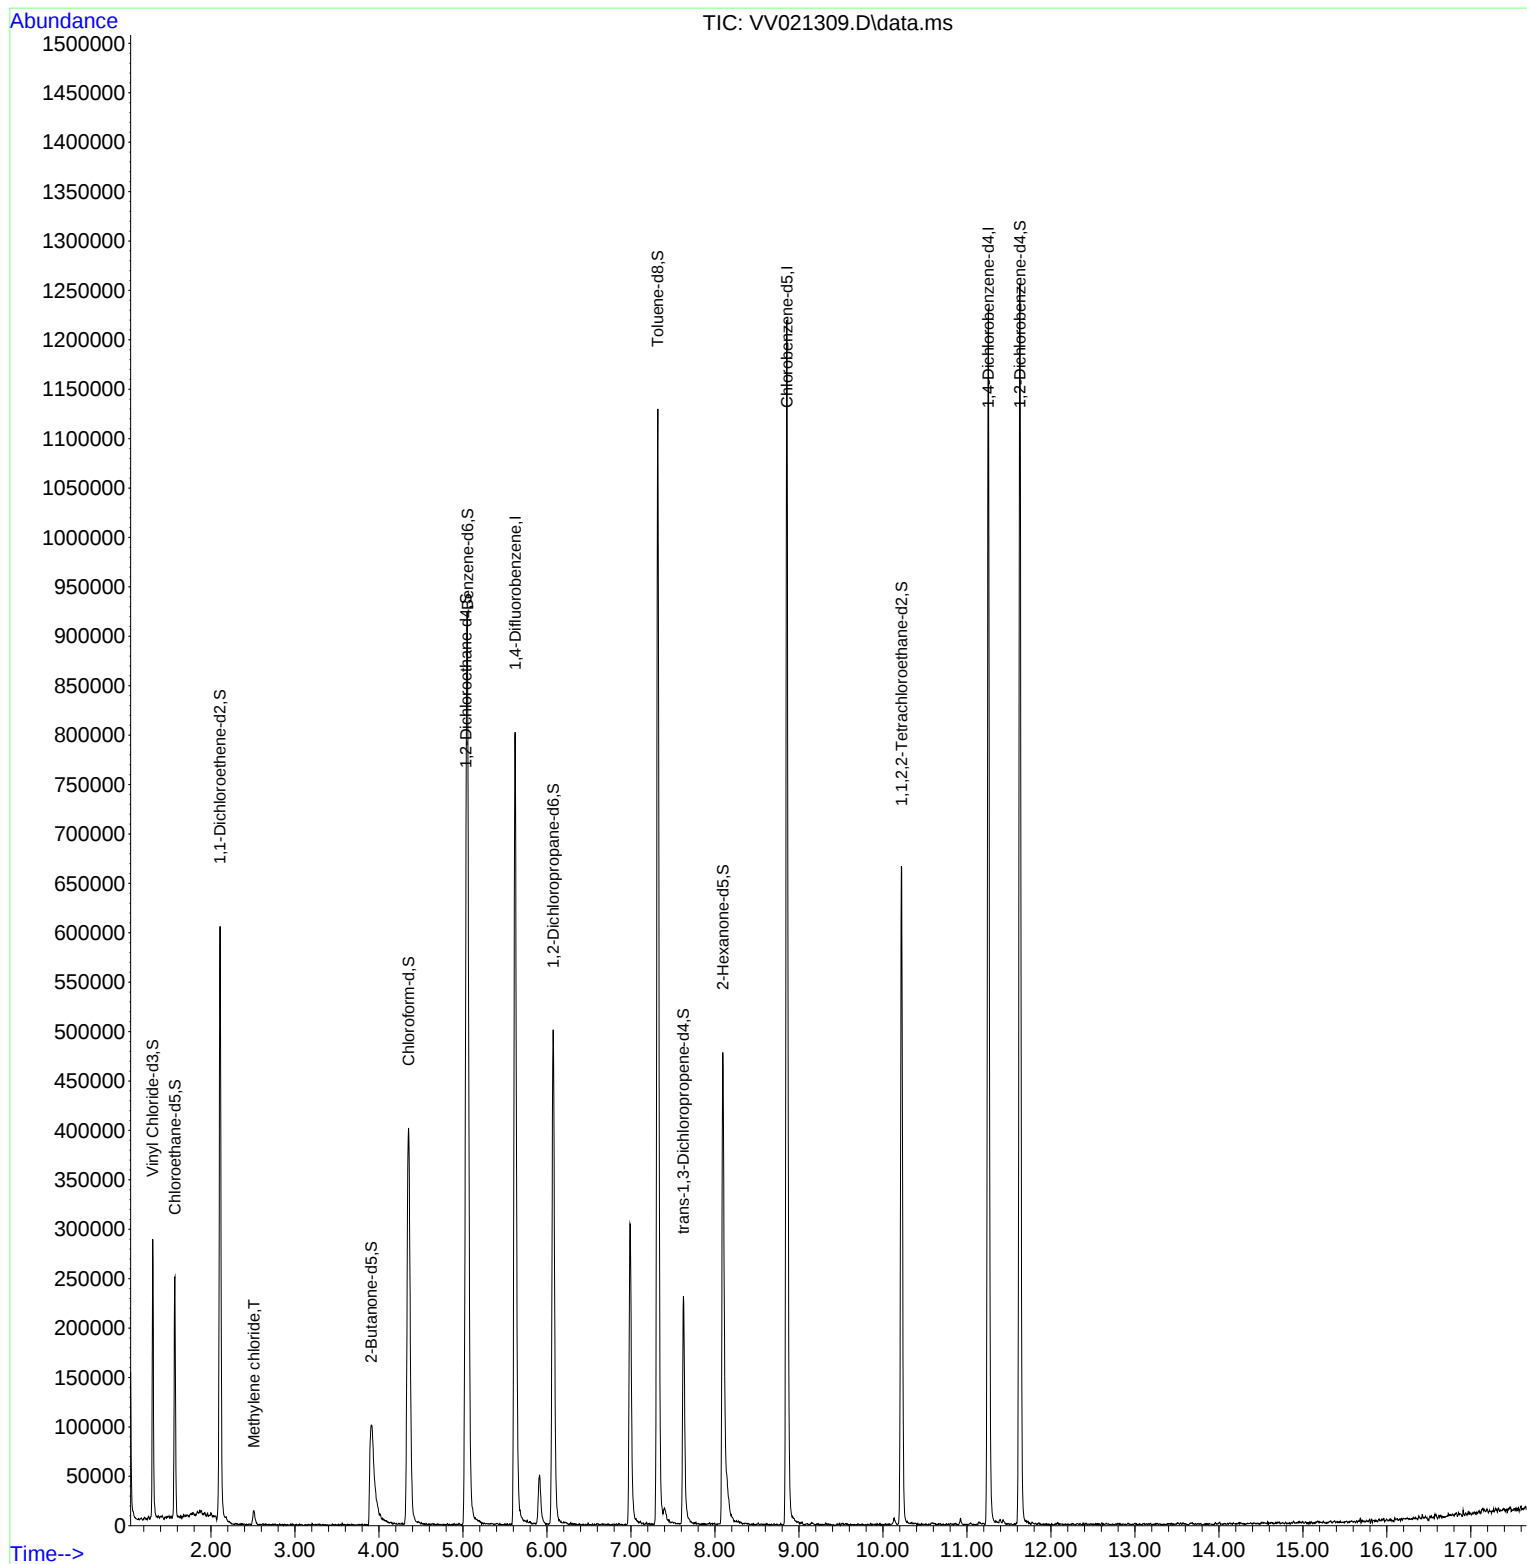

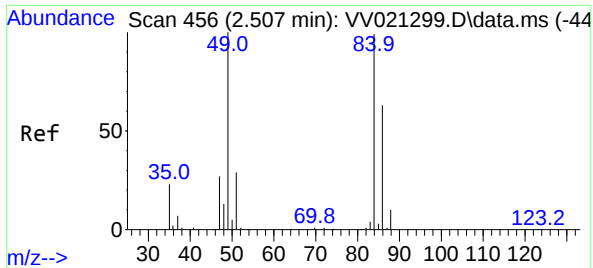

#16
Methylene chloride
Concen: 1.39 ug/L
RT: 2.513 min Scan# 458
Delta R.T. 0.006 min
Lab File: VV021309.D
Acq: 06 May 2021 15:08

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 5988

Ion	Ratio	Lower	Upper
84	100		
86	64.7	44.9	83.5
49	92.3	78.1	145.1

