

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW050621\
 Data File : VW021312.D
 Acq On : 06 May 2021 17:13
 Operator : SY/MD
 Sample : M2320-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3A05

Manual Integrations
 APPROVED

MMDadoda
 5/11/2021 1:12:20 PM

Quant Time: May 07 03:58:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 07 03:56:18 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	400929	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	404836	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	210649	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	144083	81.01	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 162.02%#			
7) Chloroethane-d5	1.571	69	125592	79.02	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 158.04%#			
11) 1,1-Dichloroethene-d2	2.111	63	264765	53.36	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 106.72%			
21) 2-Butanone-d5	3.899	46	194850	136.53	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 136.53%#			
24) Chloroform-d	4.355	84	391420	69.15	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 138.30%#			
26) 1,2-Dichloroethane-d4	5.037	65	310684	73.32	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 146.64%#			
32) Benzene-d6	5.056	84	670425	71.91	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 143.82%#			
36) 1,2-Dichloropropane-d6	6.075	67	172995	72.23	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 144.46%#			
41) Toluene-d8	7.320	98	700430	72.50	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 145.00%#			
43) trans-1,3-Dichloroprop...	7.625	79	119344	67.00	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 134.00%#			
47) 2-Hexanone-d5	8.095	63	141329	127.79	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 127.79%			
56) 1,1,2,2-Tetrachloroeth...	10.223	84	256332	66.88	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 133.76%#			
66) 1,2-Dichlorobenzene-d4	11.632	152	308165	74.23	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 148.46%#			
Target Compounds						Qvalue
17) trans-1,2-Dichloroethene	2.764	96	47719	18.98	ug/L	94
18) Methyl tert-butyl Ether	2.770	73	4498157	499.12	ug/L #	78
20) cis-1,2-Dichloroethene	3.915	96	33834	12.24	ug/L	89
27) 1,2-Dichloroethane	5.143	62	14460	2.77	ug/L #	66
29) Cyclohexane	4.680	56	25309	7.44	ug/L #	77
33) Benzene	5.114	78	28990	2.80	ug/L	100
34) Trichloroethene	5.921	95	18500m	5.55	ug/L	
42) Toluene	7.403	91	11114	0.92	ug/L	78
52) Ethylbenzene	9.024	91	9790	0.70	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050621\
Data File : VV021312.D
Acq On : 06 May 2021 17:13
Operator : SY/MD
Sample : M2320-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
F3A05

Manual Integrations
APPROVED

MMDadoda
5/11/2021 1:12:20 PM

Quant Time: May 07 03:58:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 07 03:56:18 2021
Response via : Initial Calibration

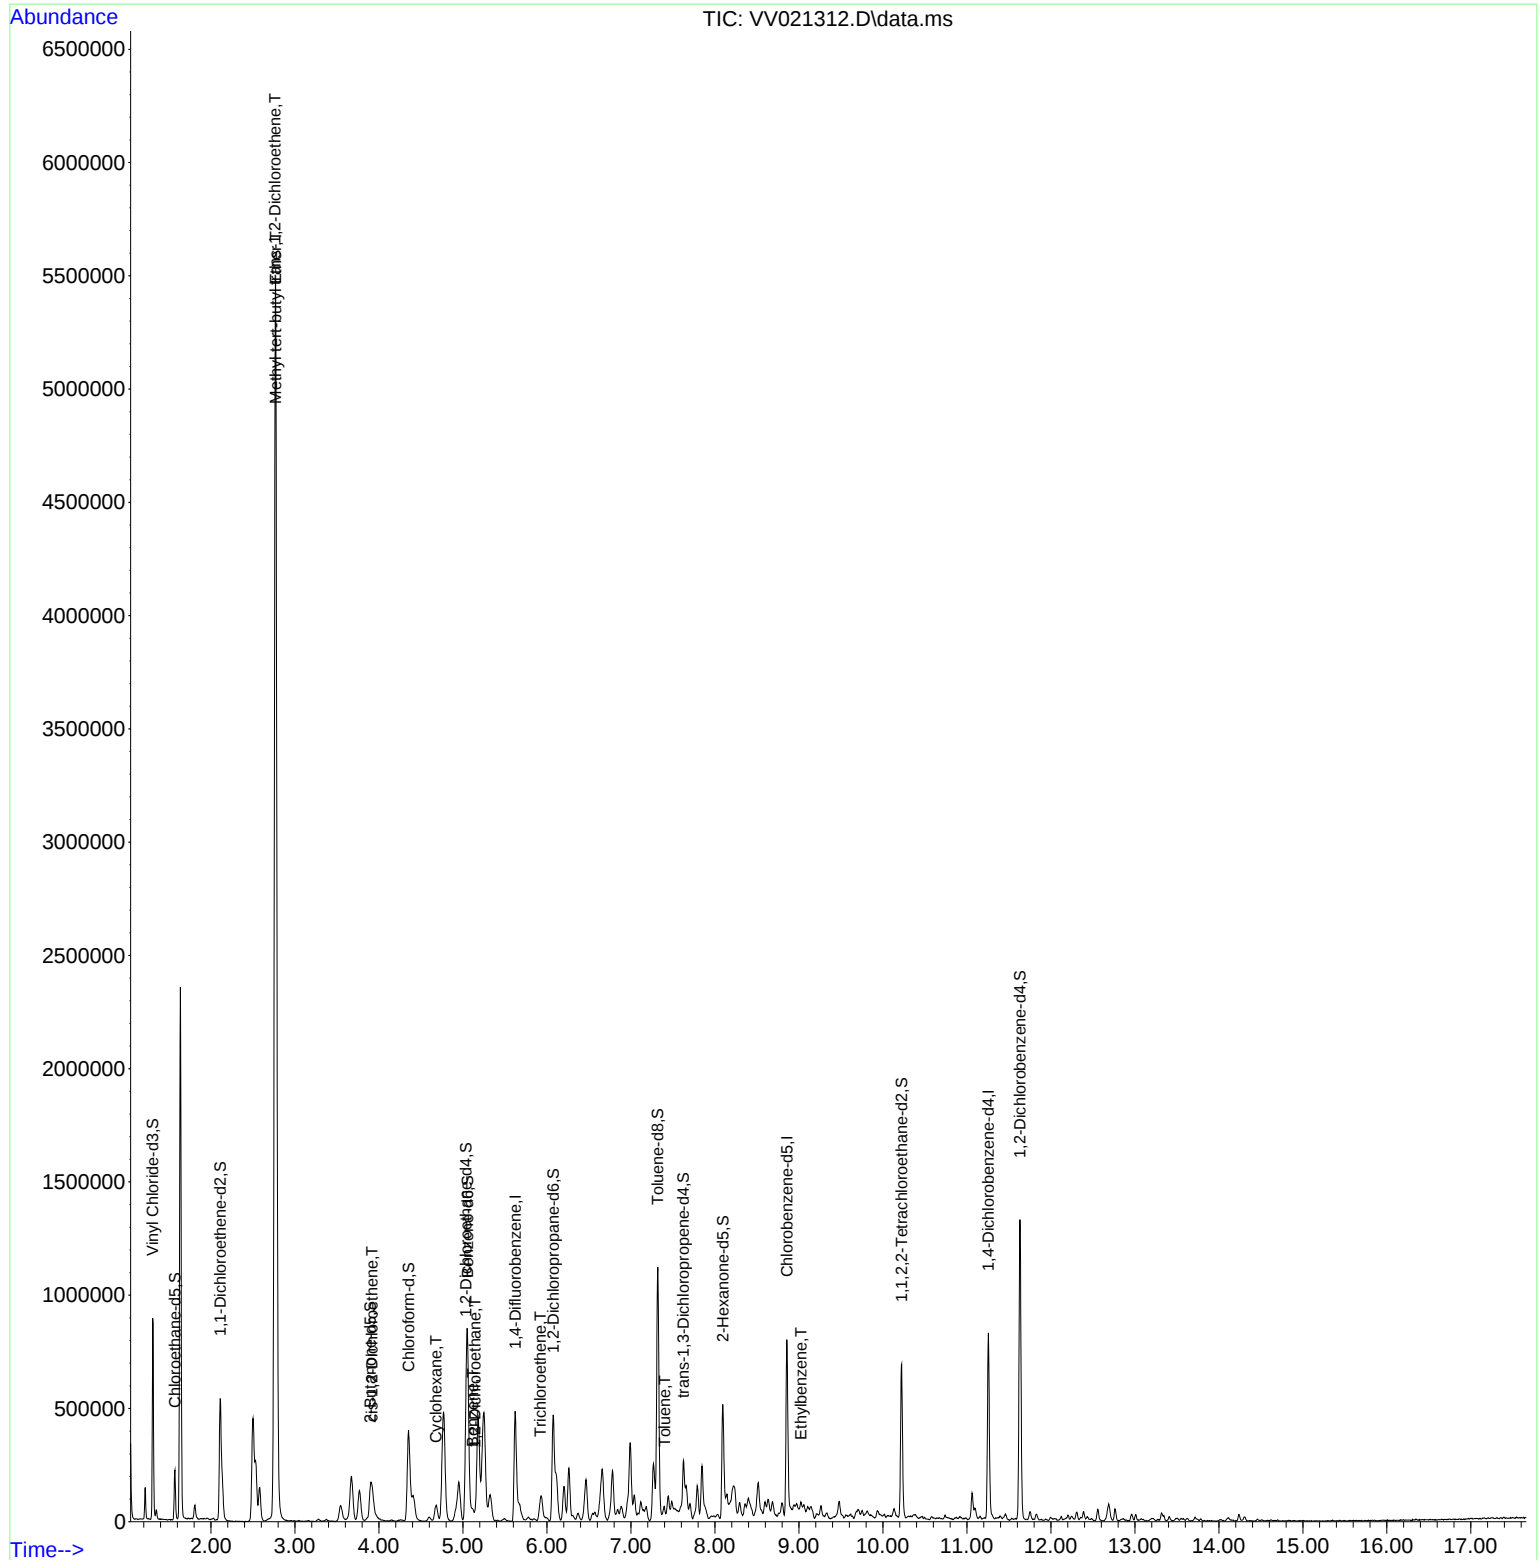

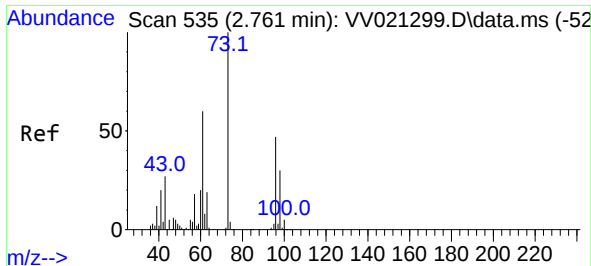





#17
trans-1,2-Dichloroethene
Concen: 18.98 ug/L
RT: 2.764 min Scan# 536
Delta R.T. 0.003 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13

Tgt Ion: 96 Resp: 47719
Ion Ratio Lower Upper
96 100
61 137.4 89.3 165.9
98 63.3 44.1 81.9

Instrument :
MSVOA_V
ClientSampleId :
F3A05




Manual Integrations
APPROVED


MMDadoda
5/11/2021 1:12:20 PM

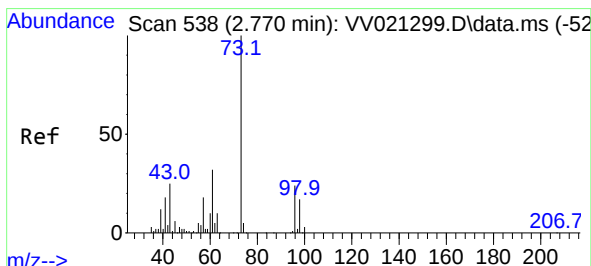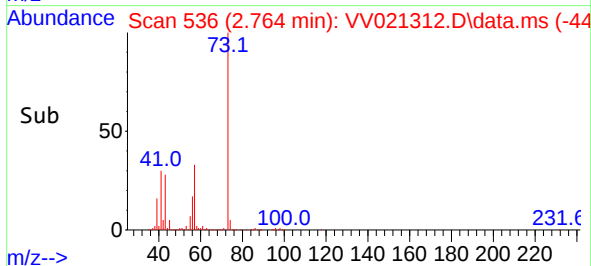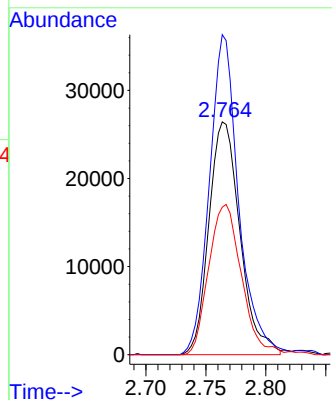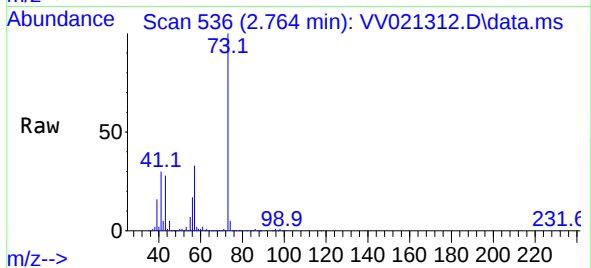

#18
Methyl tert-butyl Ether
Concen: 499.12 ug/L
RT: 2.770 min Scan# 538
Delta R.T. -0.000 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13


Tgt Ion: 73 Resp: 4498157
Ion Ratio Lower Upper
73 100
43 27.3 14.7 22.1#
57 30.7 15.9 23.9#

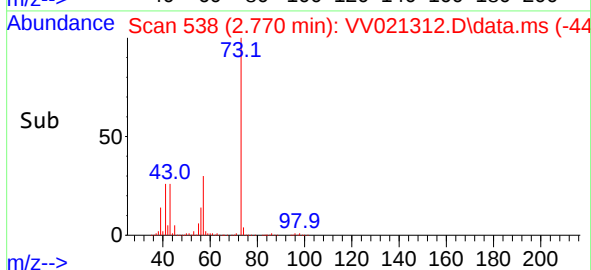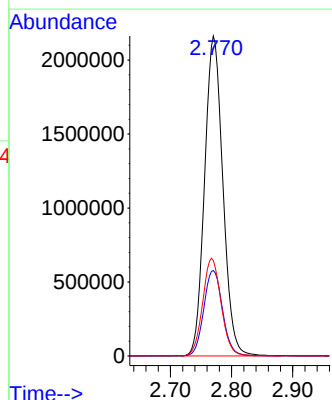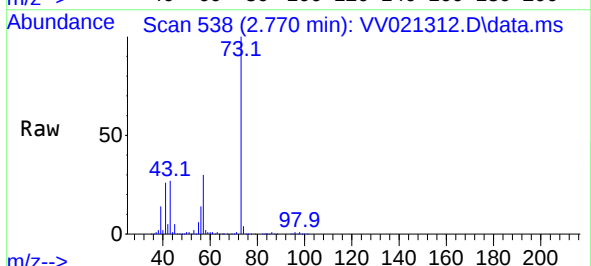

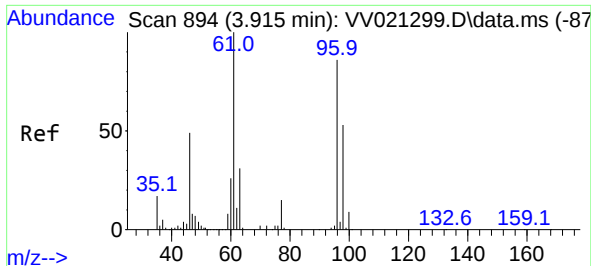

#20
cis-1,2-Dichloroethene
Concen: 12.24 ug/L
RT: 3.915 min Scan# 894
Delta R.T. -0.000 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13




Instrument :
MSVOA_V
ClientSampleId :
F3A05

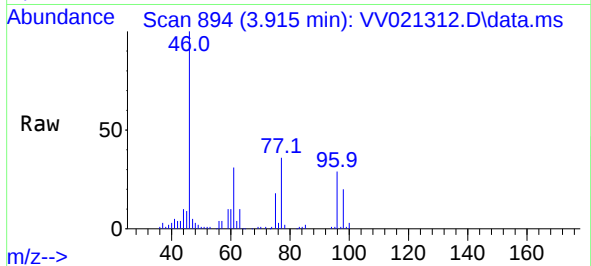


Tgt Ion: 96 Resp: 33834
Ion Ratio Lower Upper
96 100
61 108.2 84.4 156.7
68 0.0 0.0 0.0

Manual Integrations
APPROVED



MMDadoda
5/11/2021 1:12:20 PM

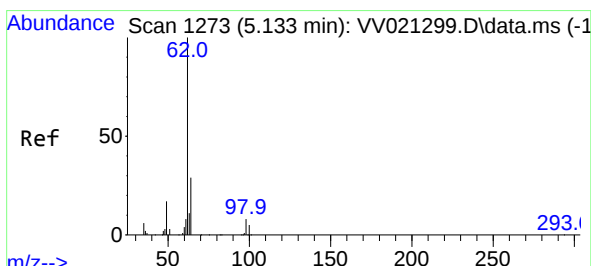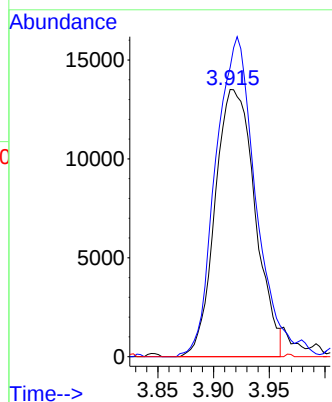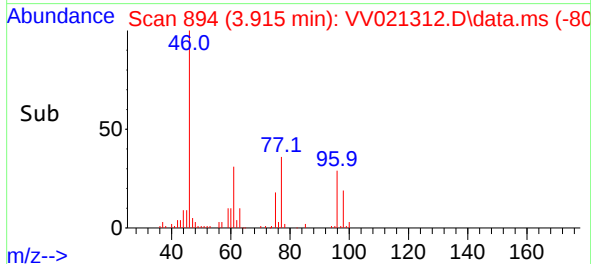


#27
1,2-Dichloroethane
Concen: 2.77 ug/L
RT: 5.143 min Scan# 1276
Delta R.T. 0.010 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13

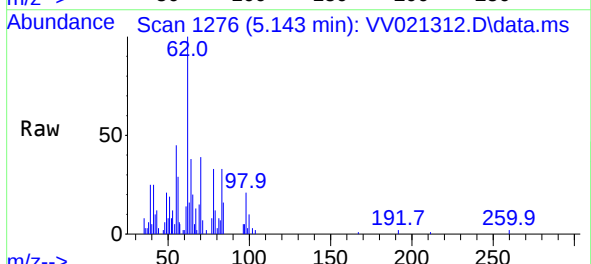


Tgt Ion: 62 Resp: 14460
Ion Ratio Lower Upper
62 100
98 20.7 6.7 10.1#

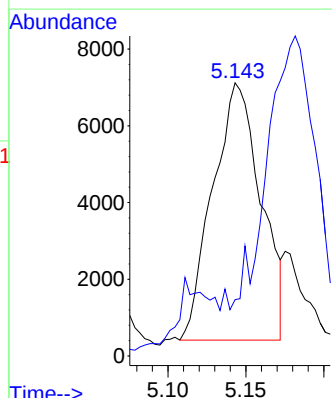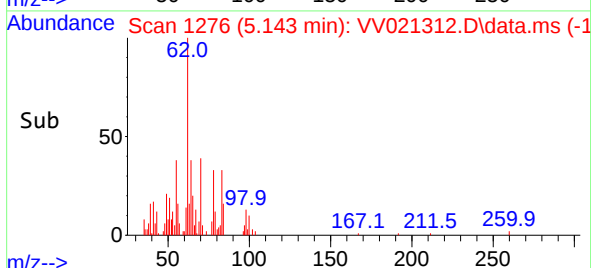

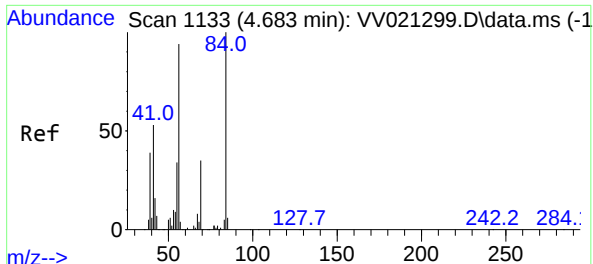

#29
Cyclohexane
Concen: 7.44 ug/L
RT: 4.680 min Scan# 1132
Delta R.T. -0.003 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13




Instrument :
MSVOA_V
ClientSampleId :
F3A05

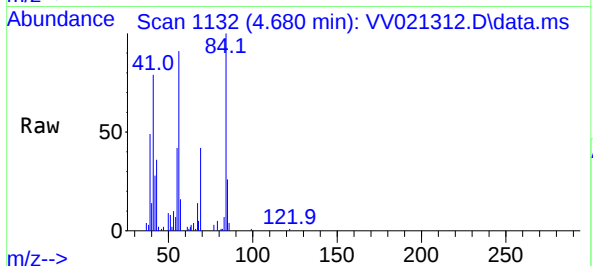

Tgt Ion: 56 Resp: 25309
Ion Ratio Lower Upper
56 100
69 44.1 25.7 38.5#
84 117.5 75.7 113.5#




Manual Integrations
APPROVED


MMDadoda
5/11/2021 1:12:20 PM

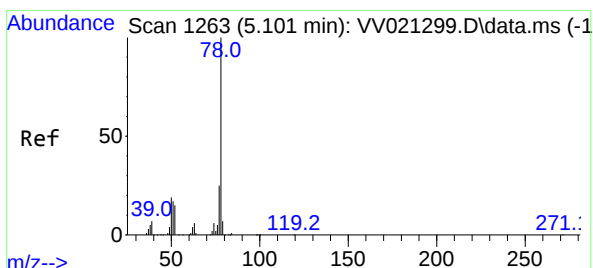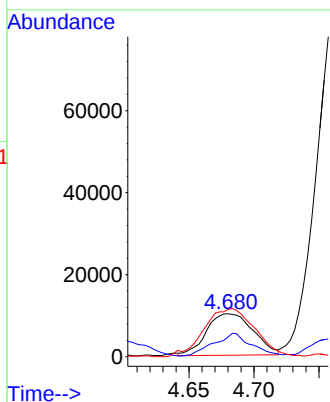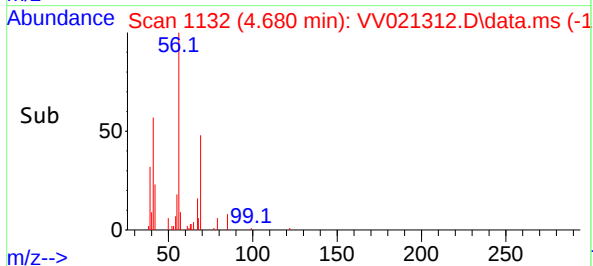

#33
Benzene
Concen: 2.80 ug/L
RT: 5.114 min Scan# 1267
Delta R.T. 0.013 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13

Tgt Ion: 78 Resp: 28990

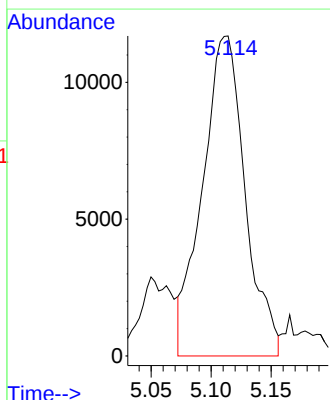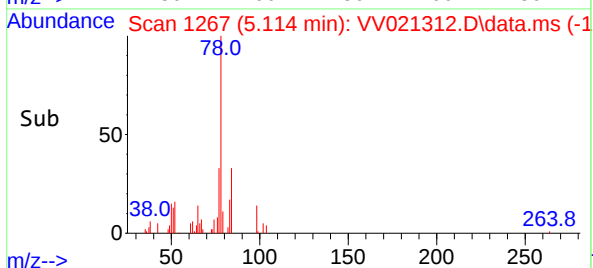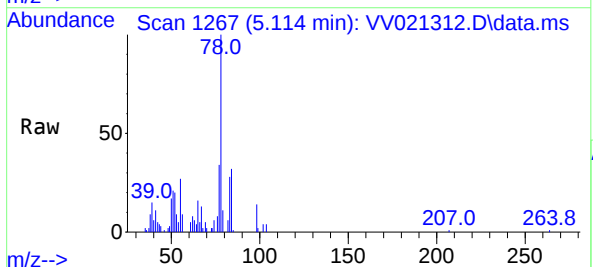

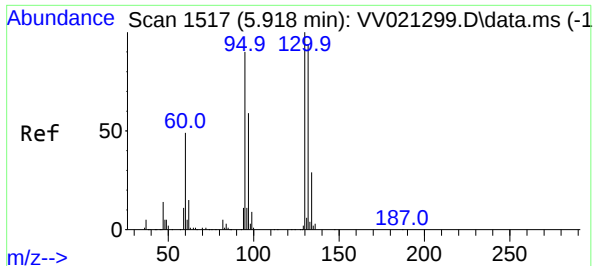





#34
Trichloroethene
Concen: 5.55 ug/L m
RT: 5.921 min Scan# 1518
Delta R.T. 0.003 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13

Tgt Ion: 95 Resp: 18500
Ion Ratio Lower Upper
95 100
97 59.8 45.5 84.5
132 109.7 71.0 131.8
130 110.5 75.7 140.7

Instrument :
MSVOA_V
ClientSampleId :
F3A05




Manual Integrations
APPROVED


MMDadoda
5/11/2021 1:12:20 PM

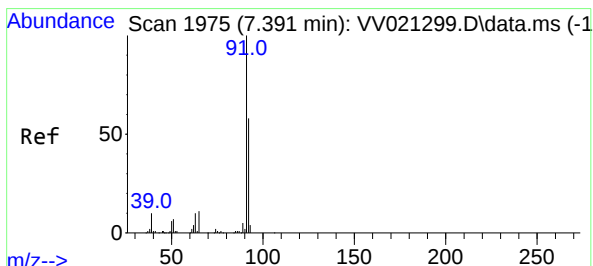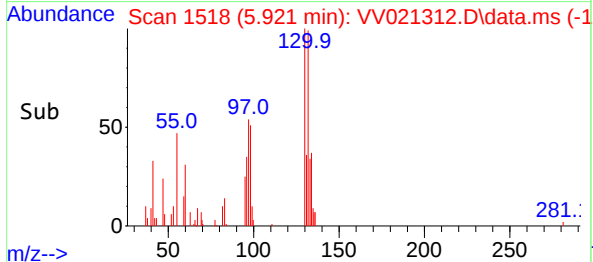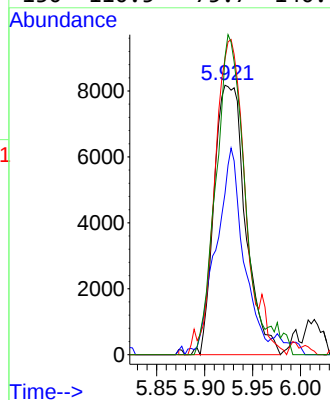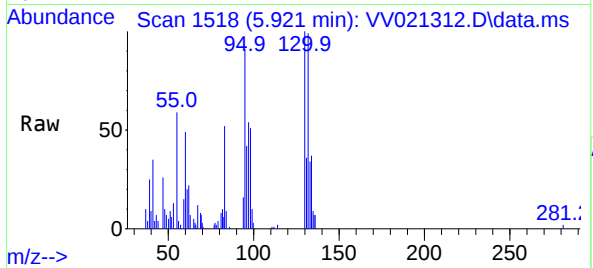

#42
Toluene
Concen: 0.92 ug/L
RT: 7.403 min Scan# 1979
Delta R.T. 0.013 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13


Tgt Ion: 91 Resp: 11114
Ion Ratio Lower Upper
91 100
92 42.0 41.0 76.2

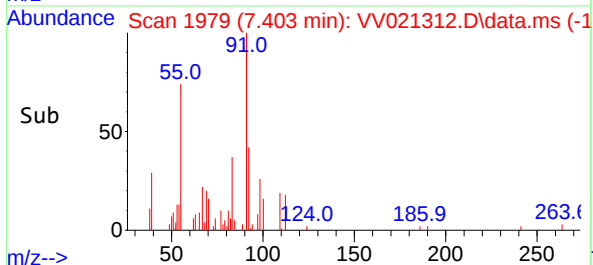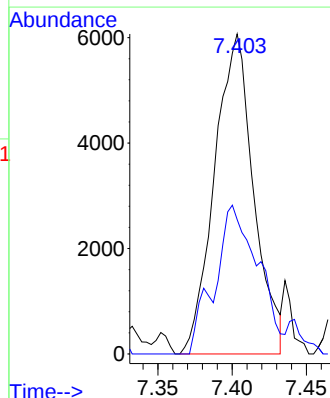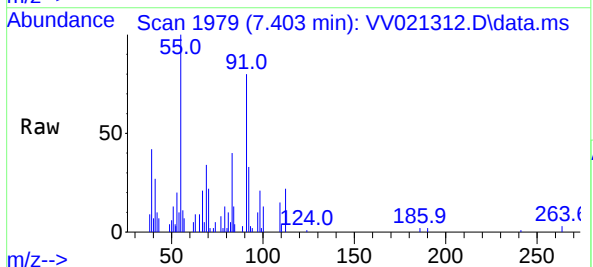

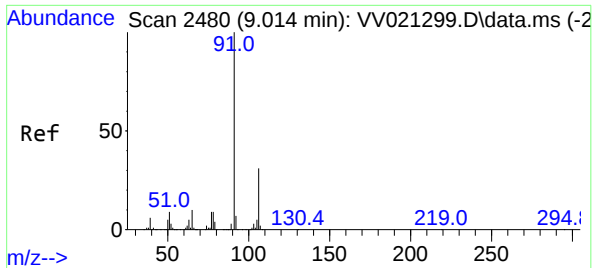

#52
Ethylbenzene
Concen: 0.70 ug/L
RT: 9.024 min Scan# 2483
Delta R.T. 0.010 min
Lab File: VV021312.D
Acq: 06 May 2021 17:13

Instrument :
MSVOA_V
ClientSampleId :
F3A05

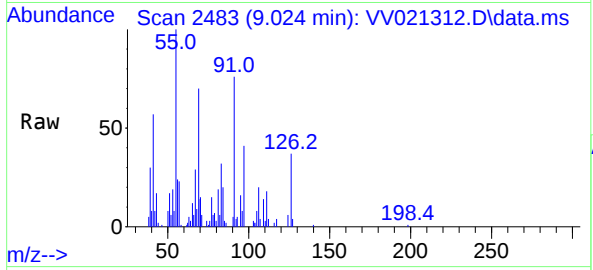

Tgt Ion: 91 Resp: 9790
Ion Ratio Lower Upper
91 100
106 25.7 21.8 40.4

Manual Integrations
APPROVED

MMDadoda
5/11/2021 1:12:20 PM

