

Data File : VV010721.D
Acq On : 08 May 2019 10:07
Operator : SY/MD
Sample : K2690-23MSD
Misc : 5.29G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A5167MSD

Quant Time: May 09 02:27:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
Quant Title : VOC Analysis
QLast Update : Thu May 09 02:24:26 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	105379	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	101759	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	39585	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	25798	15.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.04%
7) Chloroethane-d5	1.56	69	26597	19.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.96%
10) 1,1-Dichloroethene-d2	2.12	63	63530	17.89	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.56%
20) 2-Butanone-d5	3.93	46	28341	57.69	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.38%
24) Chloroform-d	4.39	84	65500	22.80	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.20%
26) 1,2-Dichloroethane-d4	5.07	65	44180	24.62	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.48%
29) Benzene-d6	5.09	84	121820	22.74	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.96%
33) 1,2-Dichloropropane-d6	6.11	67	42767	25.06	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.24%
37) Toluene-d8	7.36	98	104725	20.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.68%
38) trans-1,3-Dichloropropene-	7.66	79	16008	20.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.28%
39) 2-Hexanone-d5	8.13	63	21192	59.34	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.68%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	42447	26.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.84%
61) 1,2-Dichlorobenzene-d4	11.67	152	36472	23.79	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.16%

Target Compounds


						Qvalue
12) 1,1-Dichloroethene	2.13	96	36231	21.839	ug/L	94
13) Acetone	2.18	43	5435	7.146	ug/L	95
16) Methylene chloride	2.52	84	3435	2.108	ug/L	90
34) Benzene	5.14	78	156948	26.273	ug/L	100
35) Trichloroethene	5.95	95	37589	22.464	ug/L	98
40) 1,2-Dichloropropane	6.11	63	4990	3.140	ug/L #	87
44) Toluene	7.43	91	160489	23.655	ug/L	99
52) Chlorobenzene	8.92	112	105038	23.697	ug/L	99
59) 1,2,3-Trichloropropane	11.29	75	5169	3.872	ug/L #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV010721.D
Acq On : 08 May 2019 10:07
Operator : SY/MD
Sample : K2690-23MSD
Misc : 5.29G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A5167MSD

Quant Time: May 09 02:27:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
Quant Title : VOC Analysis
QLast Update : Thu May 09 02:24:26 2019
Response via : Initial Calibration




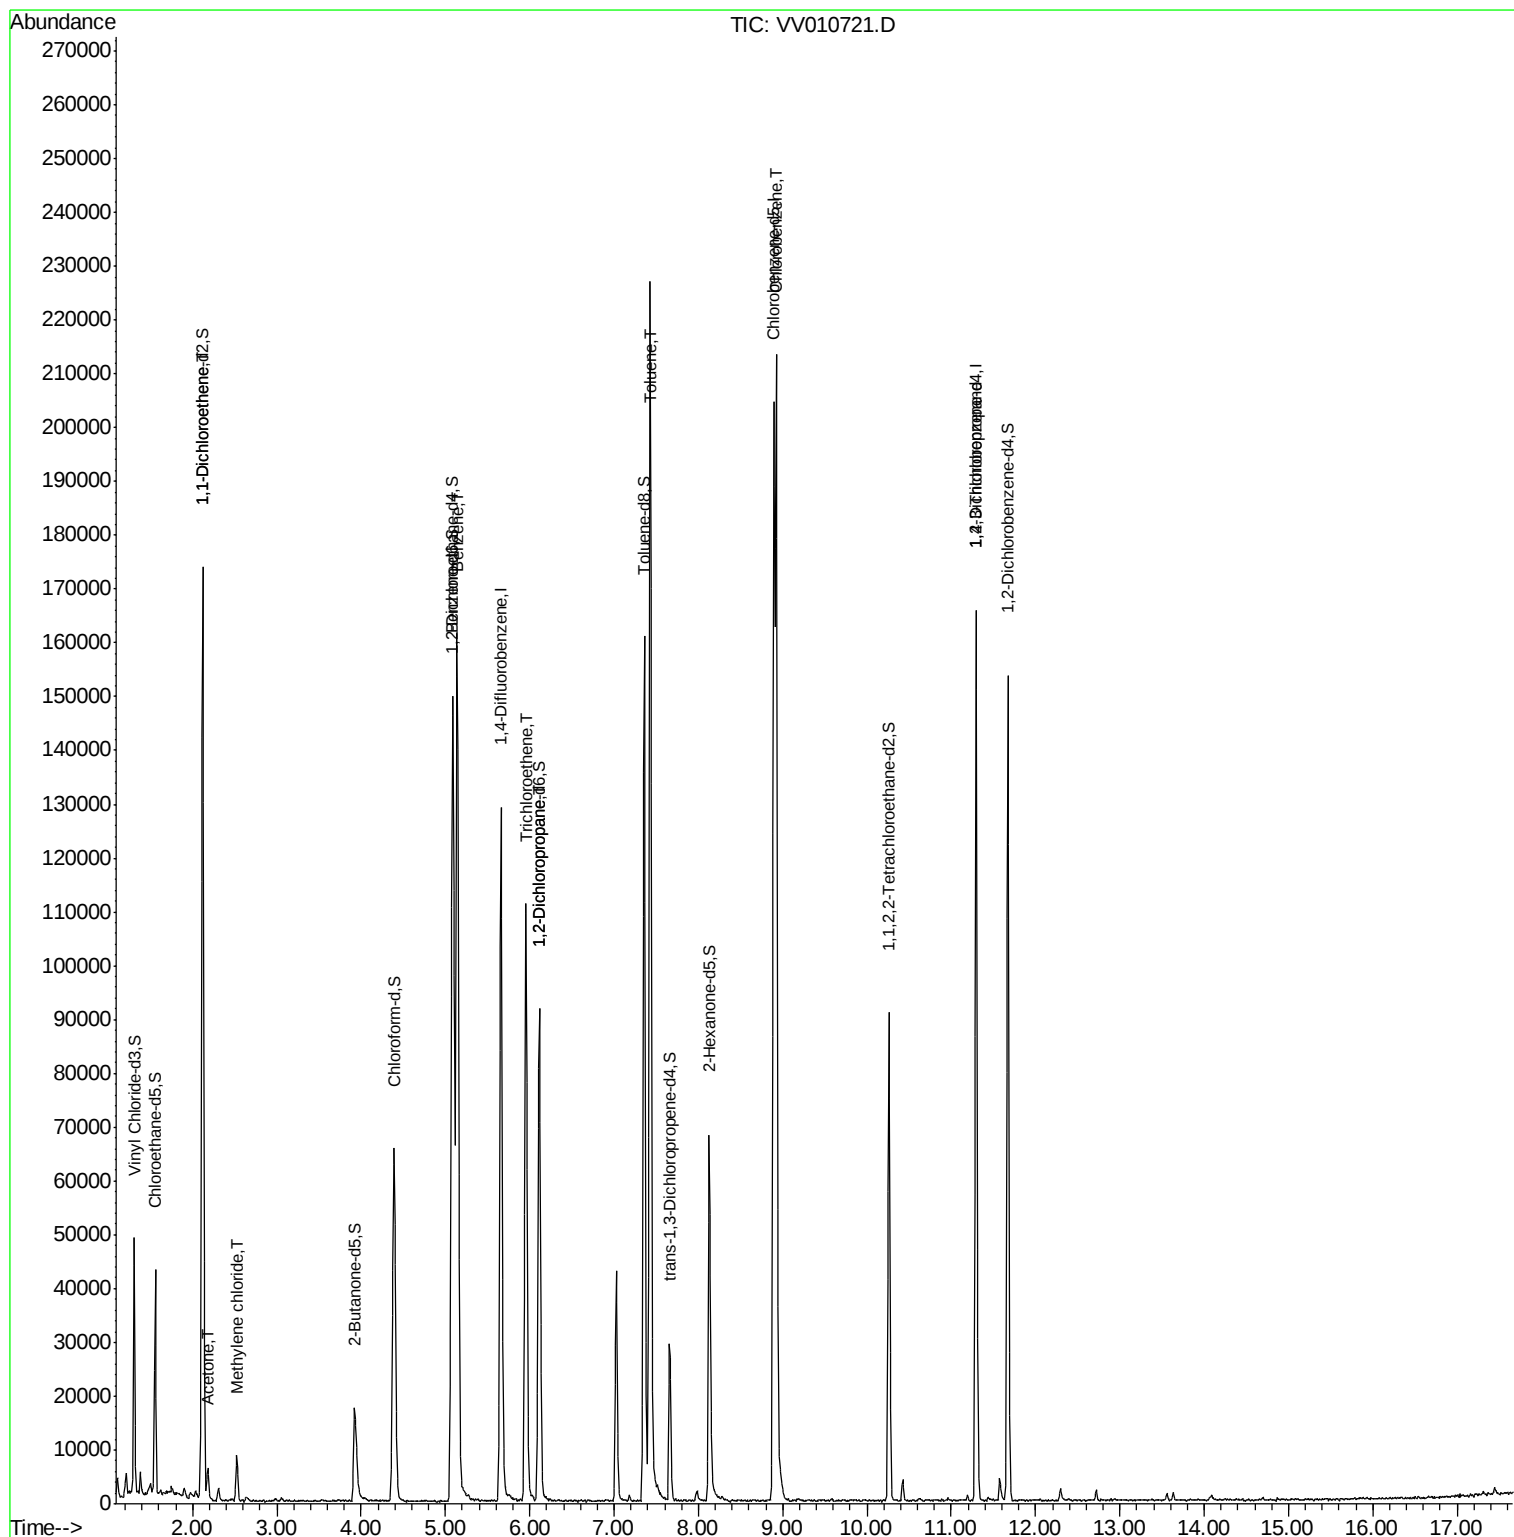


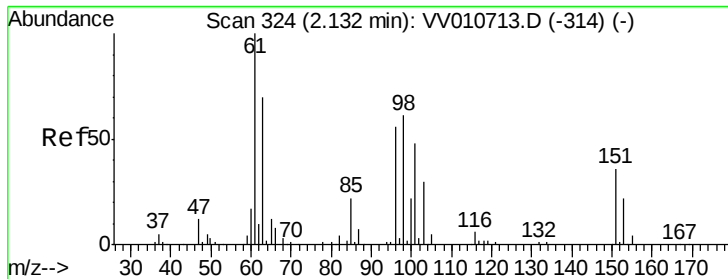

#12
 1,1-Dichloroethene
 Concen: 21.839 ug/L
 RT: 2.13 min Scan# 322
 Delta R.T. -0.01 min
 Lab File: VV010721.D
 Acq: 08 May 2019 10:07




Instrument :
 MSVOA_V
 ClientSampleId :
 A5167MSD


Tgt Ion: 96 Resp: 36231
 Ion Ratio Lower Upper
 96 100
 61 172.2 120.3 223.3
 63 103.8 82.9 153.9

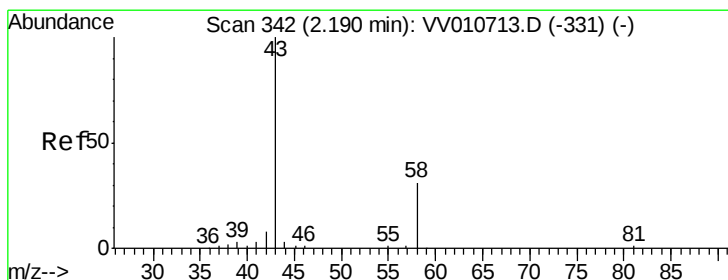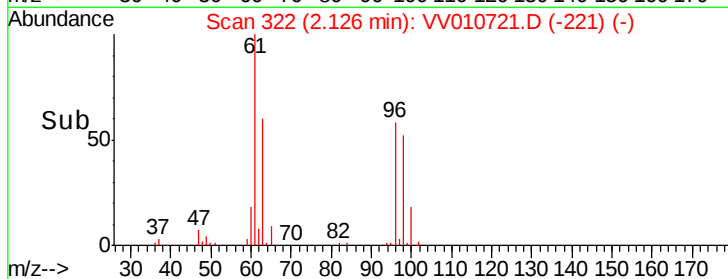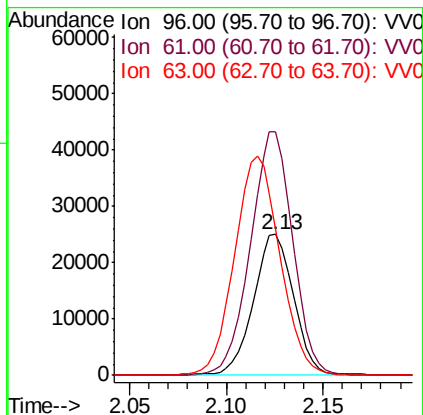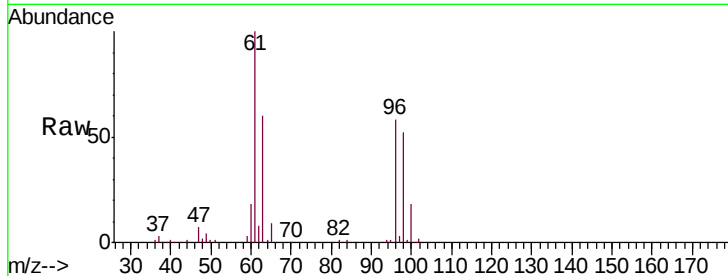

#13
 Acetone
 Concen: 7.146 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. -0.01 min
 Lab File: VV010721.D
 Acq: 08 May 2019 10:07

Tgt Ion: 43 Resp: 5435
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 63.4

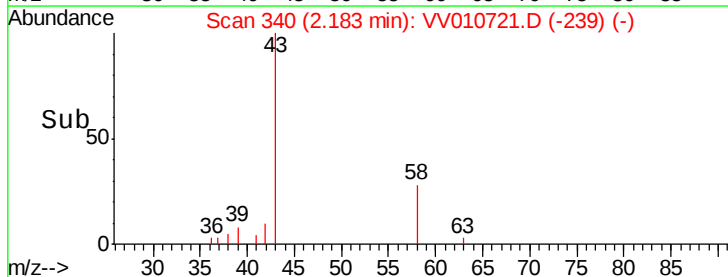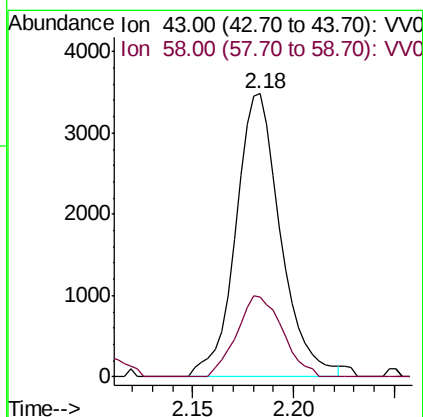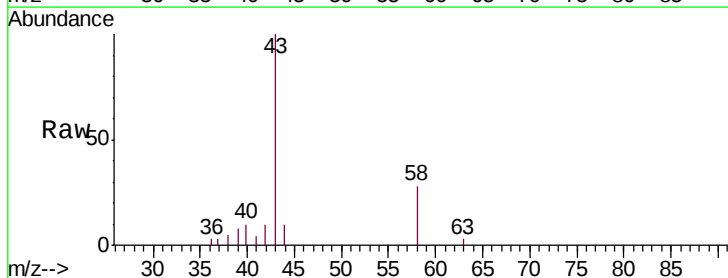

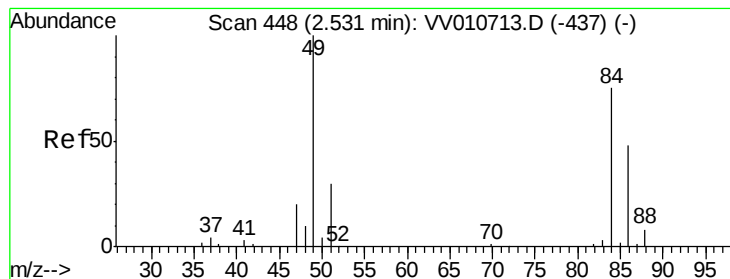

#16

Methylene chloride

Concen: 2.108 ug/L

RT: 2.52 min Scan# 446

Delta R.T. -0.01 min

Lab File: VV010721.D

Acq: 08 May 2019 10:07

Instrument :

MSVOA_V

ClientSampleId :

A5167MSD


Tgt Ion: 84 Resp: 3435

Ion Ratio Lower Upper

84 100

49 114.5 92.9 172.5




86 66.1 46.5 86.5

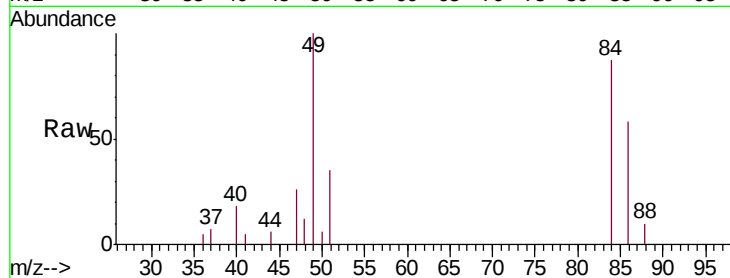

Abundance Ion 84.00 (83.70 to 84.70): VV0

Ion 49.00 (48.70 to 49.70): VV0

Ion 86.00 (85.70 to 86.70): VV0

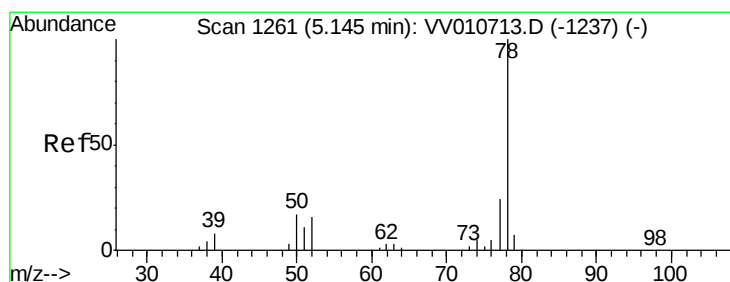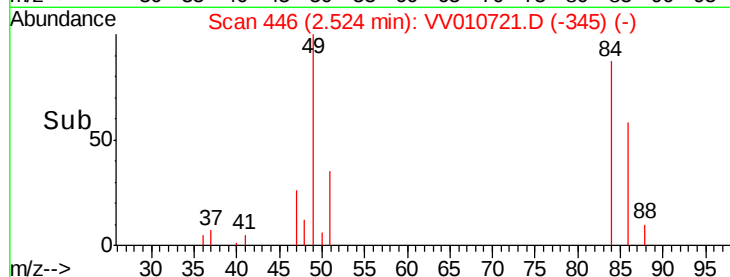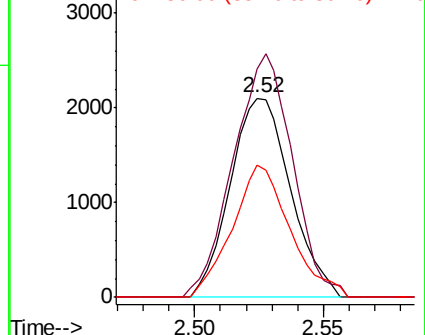

#34

Benzene

Concen: 26.273 ug/L


RT: 5.14 min Scan# 1259

Delta R.T. -0.01 min



Lab File: VV010721.D


Acq: 08 May 2019 10:07

Tgt Ion: 78 Resp: 156948

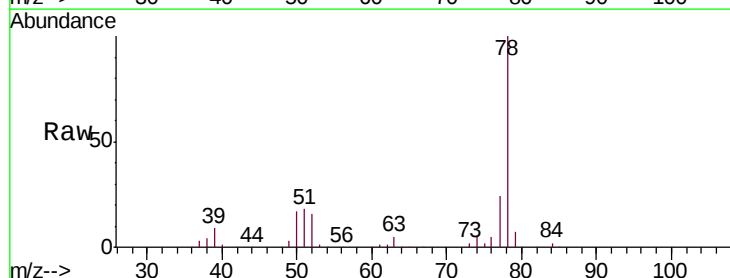

Abundance Ion 78.00 (77.70 to 78.70): VV0

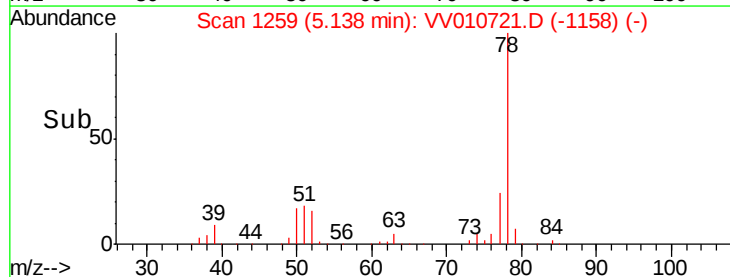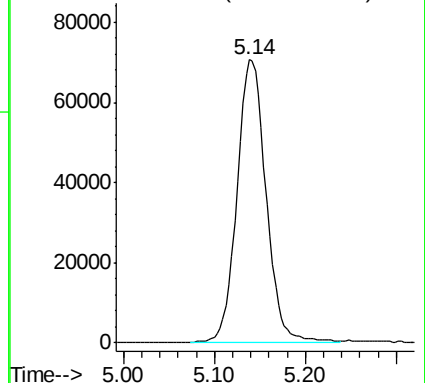

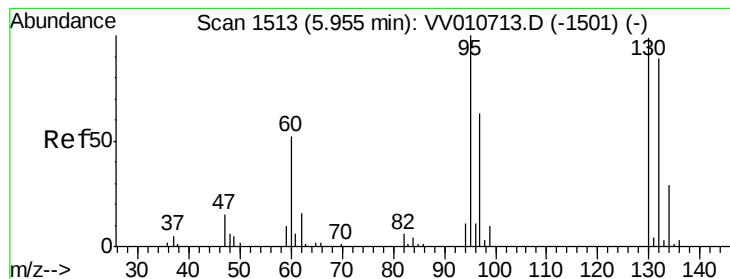

#35

Trichloroethene

Concen: 22.464 ug/L

RT: 5.95 min Scan# 1513

Delta R.T. -0.00 min

Lab File: VV010721.D

Acq: 08 May 2019 10:07

Instrument :

MSVOA_V

ClientSampleId :

A5167MSD

Tgt Ion: 95 Resp: 37589


Ion Ratio Lower Upper

95 100

97 65.4 44.3 82.3

132 91.8 62.4 115.8

130 97.6 68.5 127.3



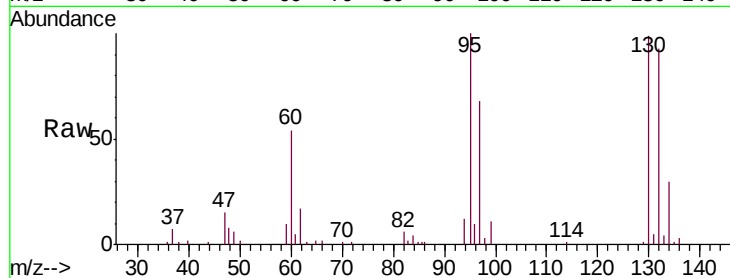


Abundance Ion 95.00 (94.70 to 95.70): VV010721.D (-1410) (-)

Ion 97.00 (96.70 to 97.70): VV010721.D (-1410) (-)

Ion 132.00 (131.70 to 132.70): VV010721.D (-1410) (-)

Ion 130.00 (129.70 to 130.70): VV010721.D (-1410) (-)

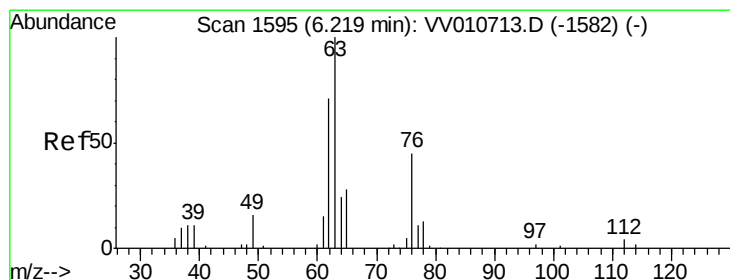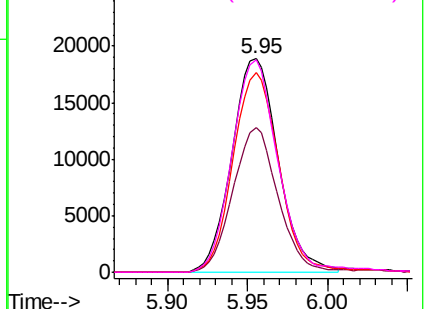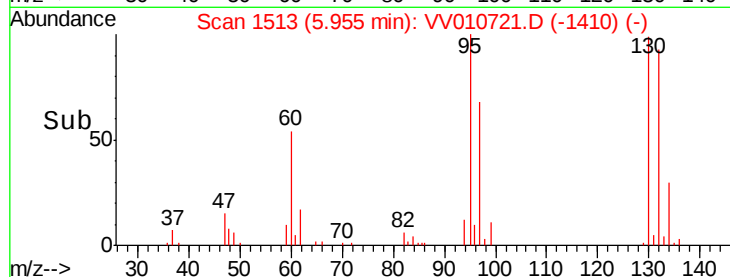

#40

1,2-Dichloropropane

Concen: 3.140 ug/L

RT: 6.11 min Scan# 1561

Delta R.T. -0.11 min

Lab File: VV010721.D


Acq: 08 May 2019 10:07

Tgt Ion: 63 Resp: 4990

Ion Ratio Lower Upper



63 100


112 0.0 3.4 5.2#

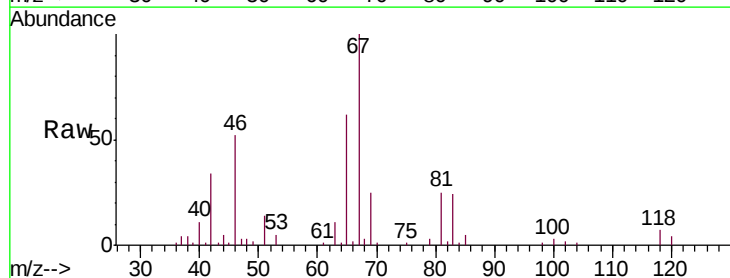

Abundance Ion 63.00 (62.70 to 63.70): VV010721.D (-1492) (-)

Ion 112.00 (111.70 to 112.70): VV010721.D (-1492) (-)

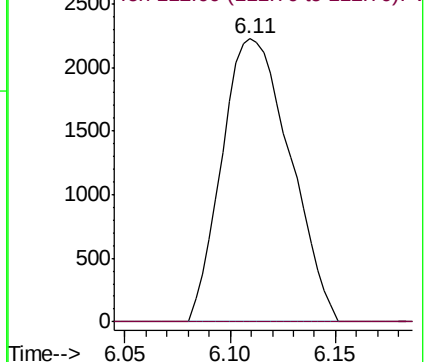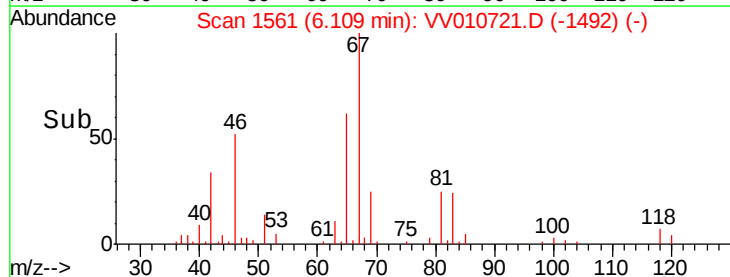

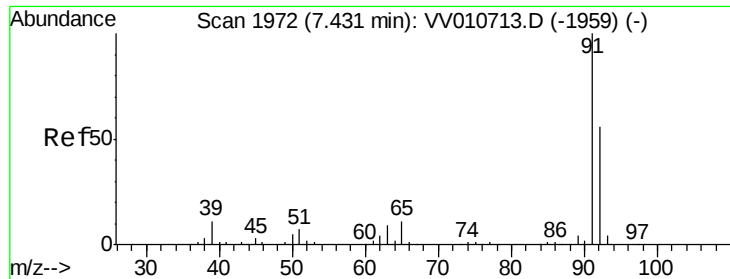

#44

Toluene

Concen: 23.655 ug/L

RT: 7.43 min Scan# 1971

Delta R.T. -0.00 min

Lab File: VV010721.D

Acq: 08 May 2019 10:07

Instrument :

MSVOA_V

ClientSampleId :


A5167MSD

Tgt Ion: 91 Resp: 160489




Ion Ratio Lower Upper

91 100

92 56.3 40.1 74.5

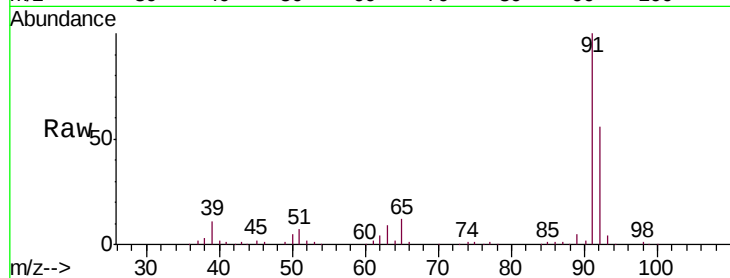

Abundance Ion 91.00 (90.70 to 91.70): VV010713.D (-1959) (-)

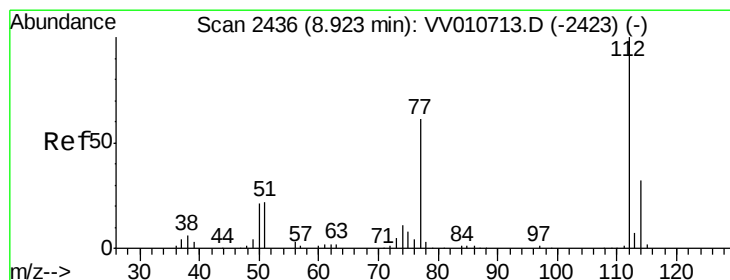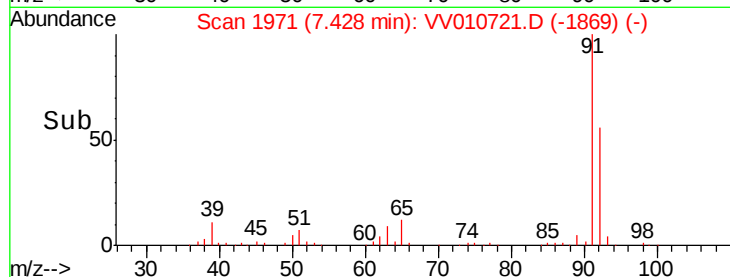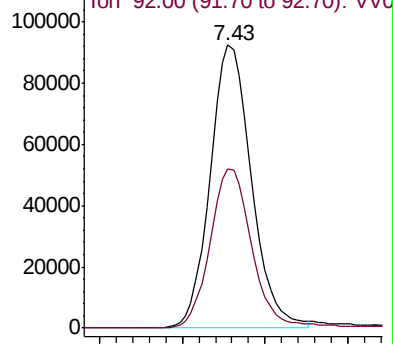

#52

Chlorobenzene

Concen: 23.697 ug/L

RT: 8.92 min Scan# 2436

Delta R.T. -0.00 min

Lab File: VV010721.D

Acq: 08 May 2019 10:07


Tgt Ion: 112 Resp: 105038

Ion Ratio Lower Upper



112 100


77 60.6 47.7 71.5

114 31.2 22.1 41.1

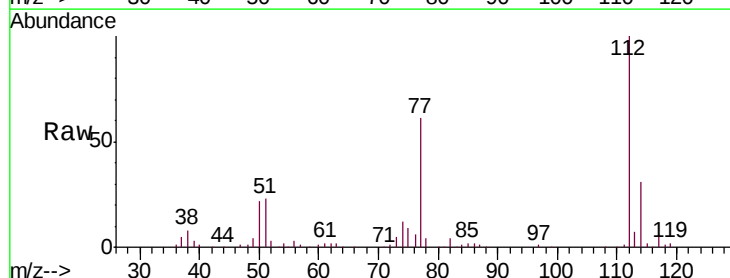

Abundance Ion 112.00 (111.70 to 112.70): VV010713.D (-2423) (-)

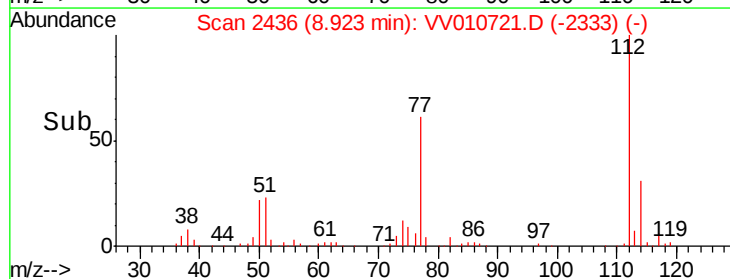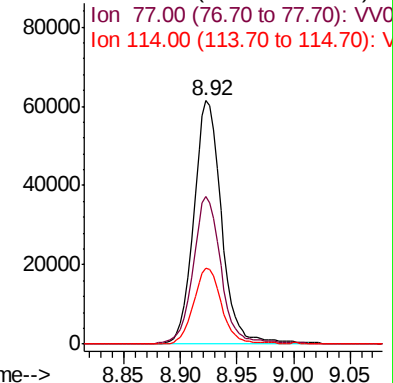

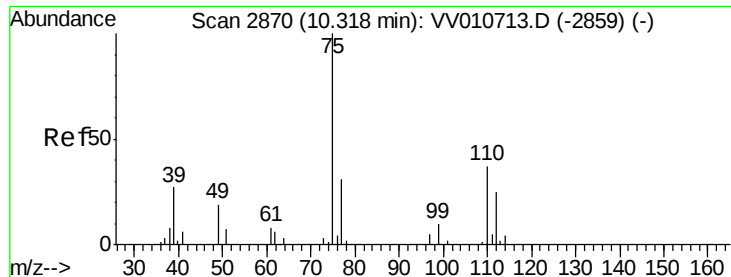

#59

1,2,3-Trichloropropane

Concen: 3.872 ug/L

RT: 11.29 min Scan# 3173

Delta R.T. 0.97 min

Lab File: VV010721.D

Acq: 08 May 2019 10:07

Instrument :

MSVOA_V

ClientSampleId :

A5167MSD

Tgt Ion: 75 Resp: 5169

Ion Ratio Lower Upper

75 100

77 40.4 25.0 37.6#

