

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050719\
 Data File : VV010747.D
 Acq On : 09 May 2019 03:29
 Operator : SY/MD
 Sample : K2692-03
 Misc : 5.86G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A5172

Quant Time: May 09 05:03:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 09 04:43:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	106853	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	105289	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40223	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	31828	19.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.68%
7) Chloroethane-d5	1.56	69	31365	22.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.84%
10) 1,1-Dichloroethene-d2	2.12	63	52653	14.62	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.48%
20) 2-Butanone-d5	3.92	46	27683	55.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.16%
24) Chloroform-d	4.39	84	75389	25.88	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.52%
26) 1,2-Dichloroethane-d4	5.07	65	50694	27.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.44%
29) Benzene-d6	5.09	84	137532	24.82	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.28%
33) 1,2-Dichloropropane-d6	6.11	67	47762	27.05	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.20%
37) Toluene-d8	7.36	98	115509	21.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.08%
38) trans-1,3-Dichloropropene-	7.66	79	18065	22.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.76%
39) 2-Hexanone-d5	8.13	63	20239	54.77	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.54%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	43833	26.41	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.64%
61) 1,2-Dichlorobenzene-d4	11.67	152	39043	25.06	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.24%


Target Compounds					Ovalue
13) Acetone	2.18	43	3678	4.769 ug/L	94




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050719\
Data File : VV010747.D
Acq On : 09 May 2019 03:29
Operator : SY/MD
Sample : K2692-03
Misc : 5.86G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A5172

Quant Time: May 09 05:03:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
Quant Title : VOC Analysis
QLast Update : Thu May 09 04:43:30 2019
Response via : Initial Calibration

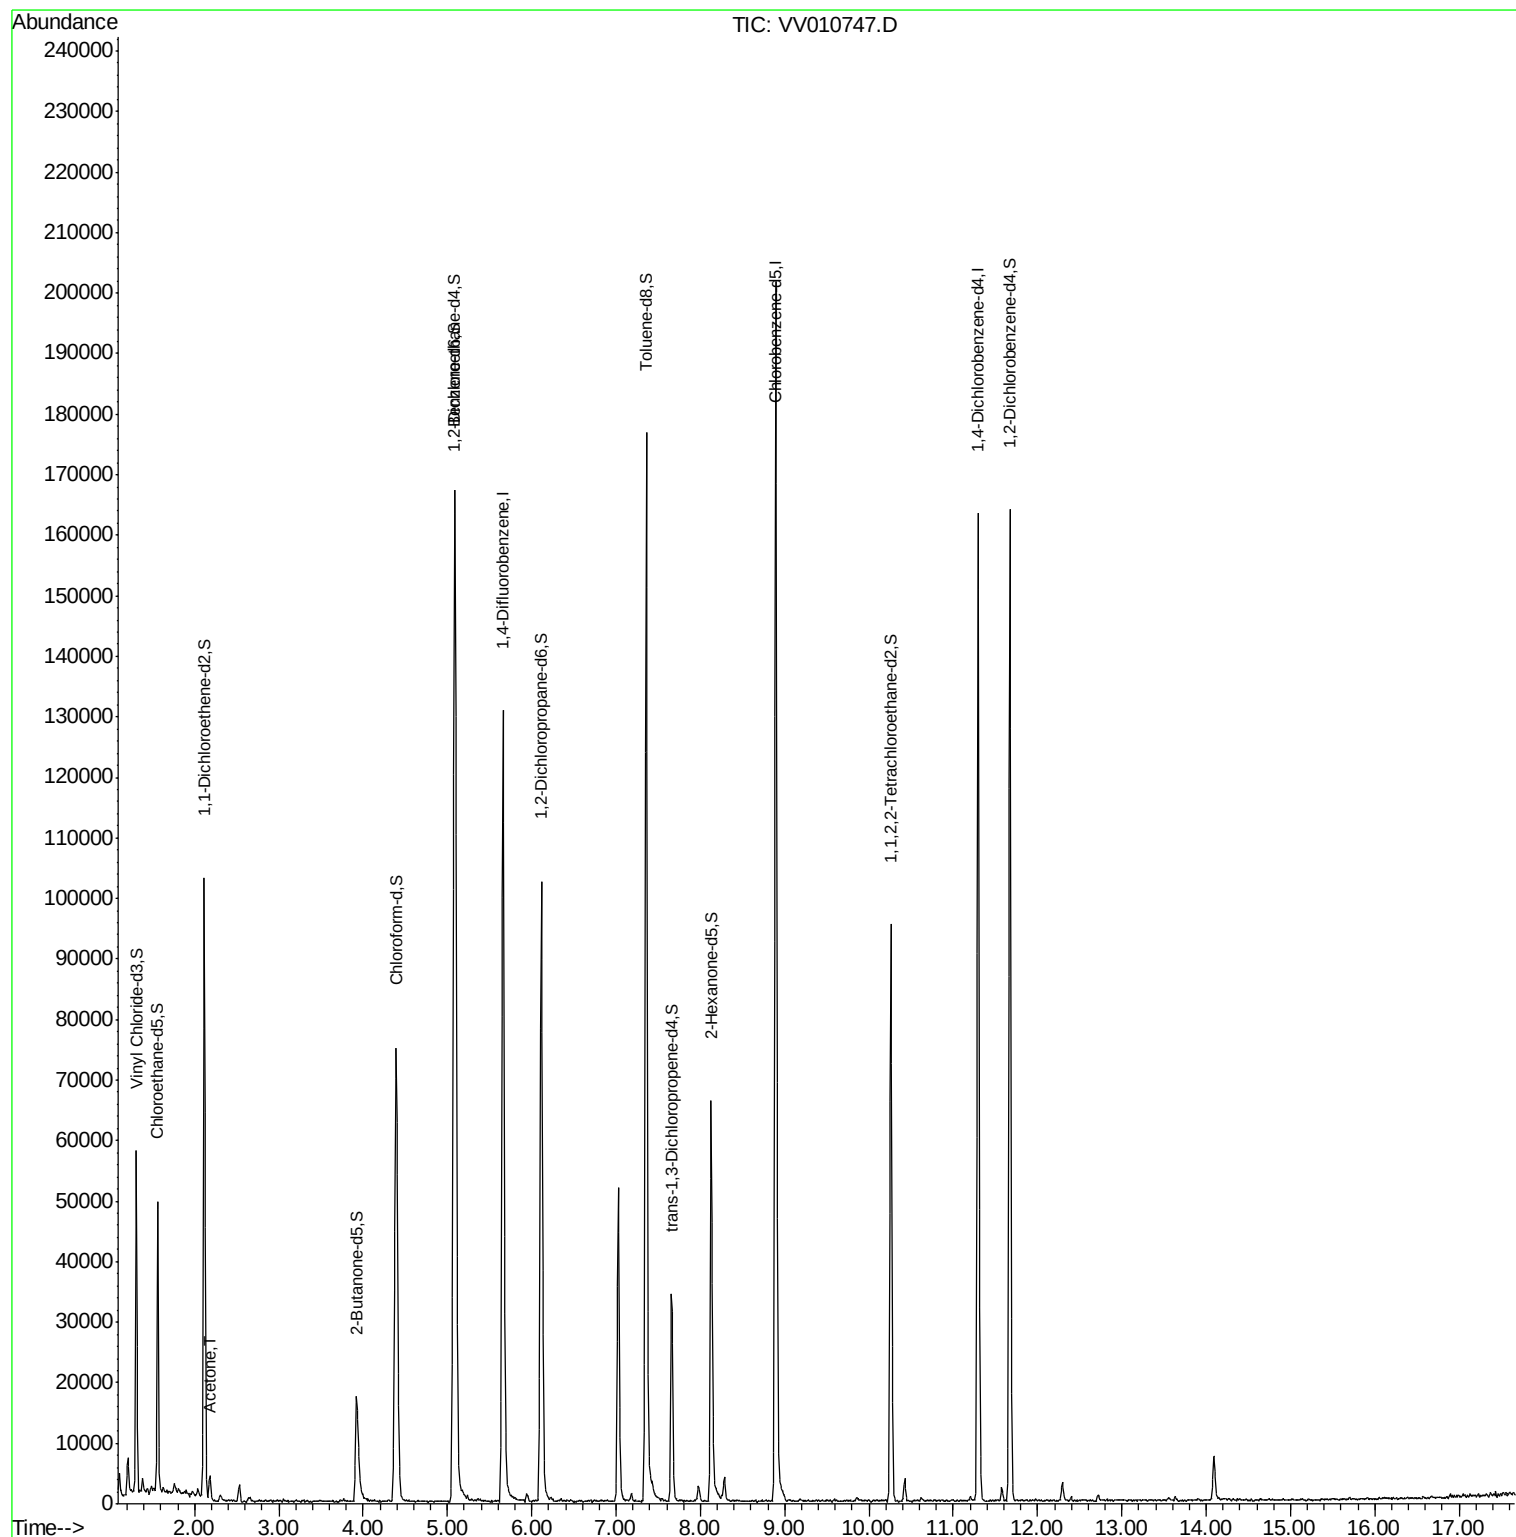

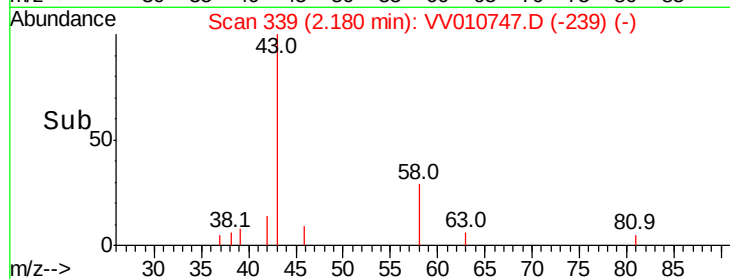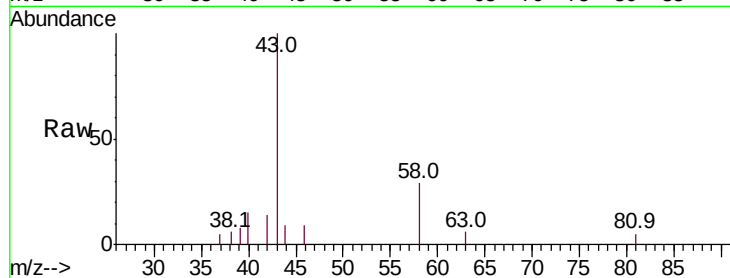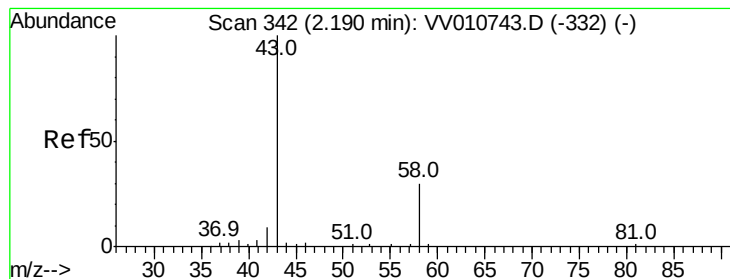

#13

Acetone

Concen: 4.769 ug/L

RT: 2.18 min Scan# 339

Delta R.T. -0.01 min

Lab File: VV010747.D

Acq: 09 May 2019 03:29

Instrument :
MSVOA_V
ClientSampleId :
A5172

Tot Ion: 43 Resp: 3678

Ion Ratio Lower Upper

43 100

58 28.5 0.0 63.4

