


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV050719\
 Data File : VV010687.D
 Acq On : 07 May 2019 10:13
 Operator : SY/MD
 Sample : BFB95
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB95

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
 Title : VOC Analysis
 Last Update : Sat May 11 00:23:03 2019

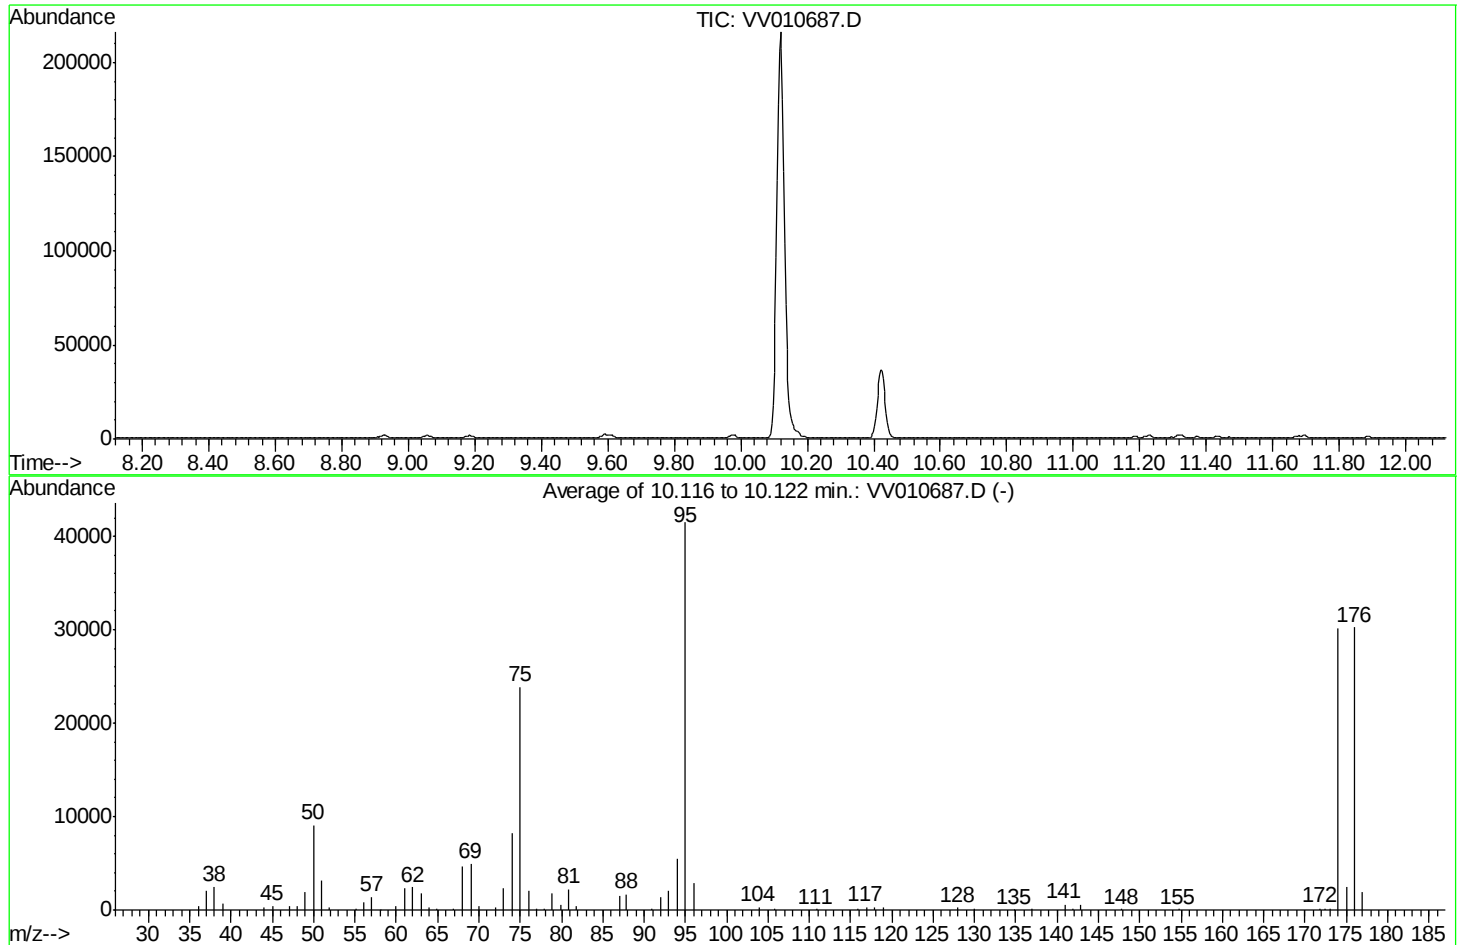

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	9080	PASS
75	95	30	80	57.5	23882	PASS
95	95	100	100	100.0	41498	PASS
96	95	5	9	6.8	2822	PASS
173	174	0.00	2	0.6	179	PASS
174	95	50	120	72.6	30125	PASS
175	174	5	9	8.0	2420	PASS
176	174	95	101	100.4	30245	PASS
177	176	5	9	6.2	1865	PASS

Scan 2796 (10.080 min): VV010687.D
BFB95

m/z	Abundance
40.00	519.0
43.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.00	487.0
37.00	2133.0
38.00	2481.0
39.00	752.0
39.90	452.0
44.00	419.0
45.00	407.0
47.00	491.0
48.00	328.0
49.00	1843.0
50.00	8960.0
51.00	2889.0
51.90	220.0
55.10	131.0
56.00	796.0
57.00	1382.0
60.00	454.0
61.00	2403.0
62.00	2479.0
63.00	2012.0
64.00	231.0
64.90	171.0
66.80	187.0
68.00	4592.0
69.00	4724.0
70.00	464.0
71.90	228.0
73.00	2196.0
74.00	8032.0
75.00	23400.0
76.10	2062.0
77.00	212.0
77.80	207.0
78.80	1813.0
79.90	485.0
80.90	2094.0
81.80	376.0
87.00	1571.0
87.90	1695.0
90.90	178.0
92.00	1466.0
93.00	2026.0
94.10	5303.0
95.00	40872.0
96.00	2871.0
103.90	247.0
105.80	202.0
110.80	132.0
115.90	182.0
116.90	300.0
118.00	236.0
118.90	296.0
128.00	205.0
129.90	203.0
136.90	163.0
140.90	641.0
141.90	128.0
142.90	444.0
147.80	141.0
154.80	111.0
171.80	240.0
173.10	538.0
174.00	29416.0
175.00	2528.0
176.00	29064.0
177.00	1742.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.00	487.0
37.00	2184.0
38.00	2580.0
39.00	752.0
40.00	436.0
44.00	445.0
45.00	421.0
47.10	456.0
48.00	373.0
49.00	1953.0
50.00	9410.0
51.00	3368.0
51.90	245.0
55.10	139.0
56.00	843.0
57.00	1426.0
58.10	102.0
60.00	434.0
61.00	2386.0
62.00	2494.0
63.00	1882.0
64.00	247.0
65.00	150.0
66.90	190.0
68.00	4805.0
69.00	5078.0
70.00	504.0
72.00	286.0
73.00	2318.0
74.00	8473.0
75.00	24664.0
76.10	2053.0
77.10	196.0
77.90	176.0
78.90	1764.0
79.90	561.0
80.90	2301.0
81.80	395.0
87.00	1616.0
87.90	1704.0
91.00	206.0
92.00	1476.0
93.00	2087.0
94.00	5677.0
95.00	42792.0
96.00	2935.0
103.90	300.0
105.70	212.0
110.90	115.0
115.90	187.0
116.90	365.0
117.90	234.0
118.90	338.0
128.00	247.0
129.90	174.0
136.90	174.0
140.90	637.0
141.90	111.0
142.80	511.0
147.80	135.0
154.70	123.0
174.00	31088.0
175.00	2518.0
176.00	31384.0
177.00	1934.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.00	445.0
37.00	2066.0
38.00	2357.0
39.00	746.0
39.90	460.0
44.00	403.0
45.00	448.0
47.10	374.0
48.10	349.0
49.00	1882.0
50.00	8872.0
51.00	3333.0
51.90	217.0
55.00	131.0
56.00	820.0
57.00	1312.0
58.10	108.0
60.00	392.0
61.00	2227.0
62.00	2331.0
63.00	1589.0
64.00	206.0
65.00	146.0
66.90	176.0
68.00	4737.0
69.00	5011.0
70.00	469.0
71.90	377.0
73.00	2328.0
74.00	8211.0
75.00	23584.0
76.10	1933.0
77.10	203.0
77.90	150.0
78.90	1705.0
79.90	566.0
80.90	2187.0
81.90	440.0
87.00	1474.0
87.90	1662.0
91.00	217.0
92.00	1362.0
93.00	1913.0
94.00	5465.0
95.00	40832.0
96.00	2662.0
103.90	311.0
105.80	207.0
115.80	195.0
116.90	361.0
117.80	221.0
118.90	341.0
128.00	239.0
129.90	161.0
134.80	104.0
136.90	149.0
140.90	542.0
142.80	513.0
147.80	104.0
154.70	113.0
171.90	200.0
172.50	266.0
174.00	29872.0
175.00	2216.0
176.00	30288.0
177.00	1921.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95