
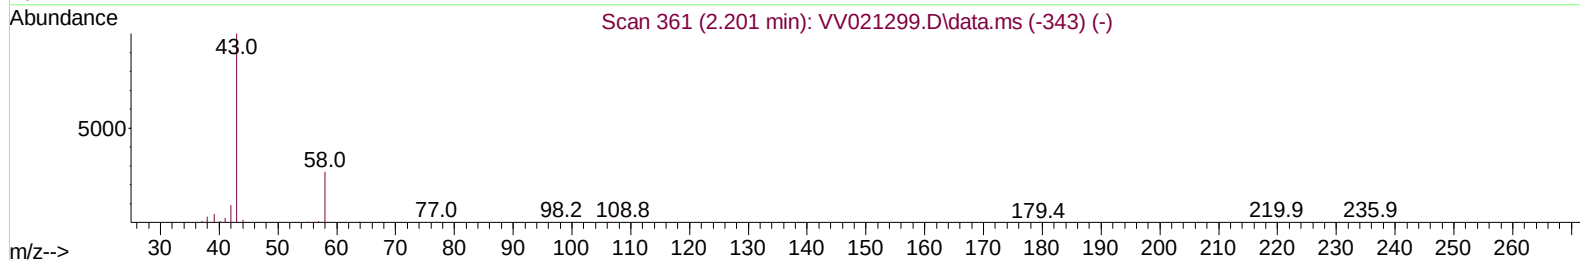
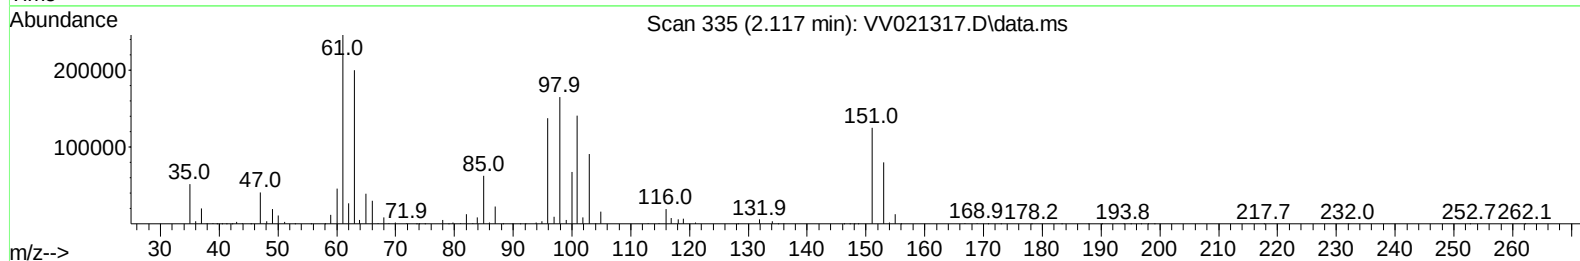


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021317.D
 Acq On : 07 May 2021 11:12
 Operator : SY/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: May 08 00:32:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 07 03:56:18 2021
 Response via : Initial Calibration

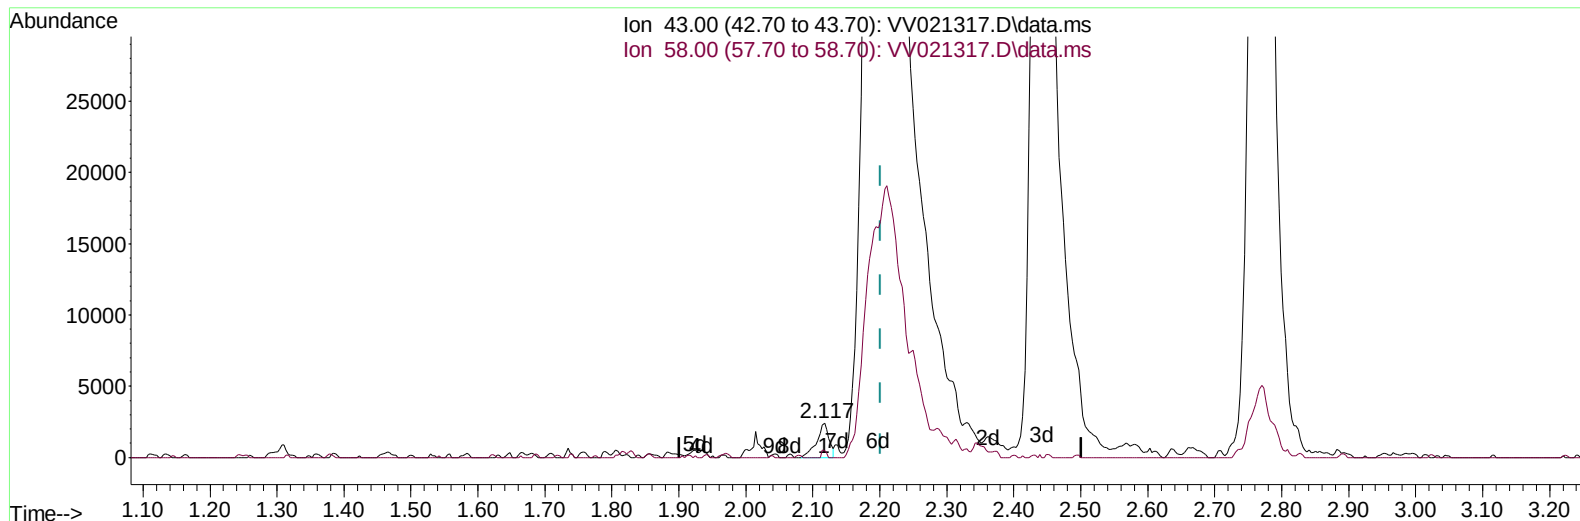

TIC: VV021317.D\data.ms

(13) Acetone (T)**2.117min (-0.084) 1.07 ug/L****response 3054**

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	8.02
0.00	0.00	0.00
0.00	0.00	0.00