
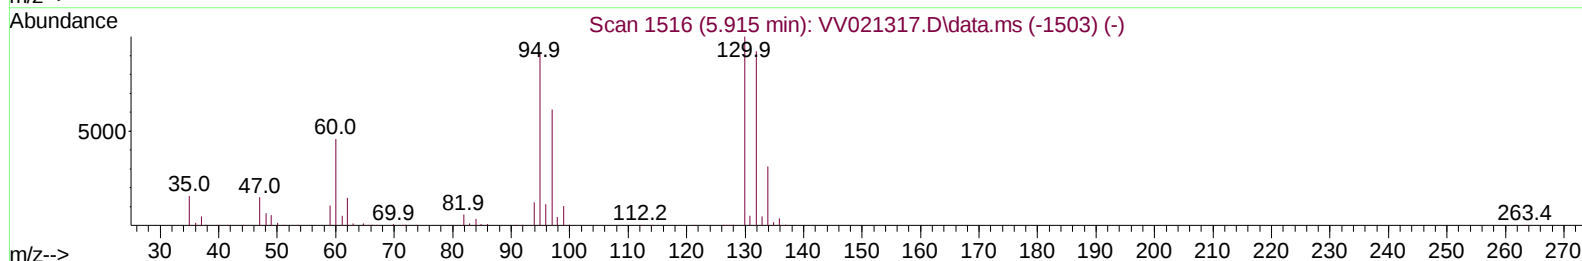
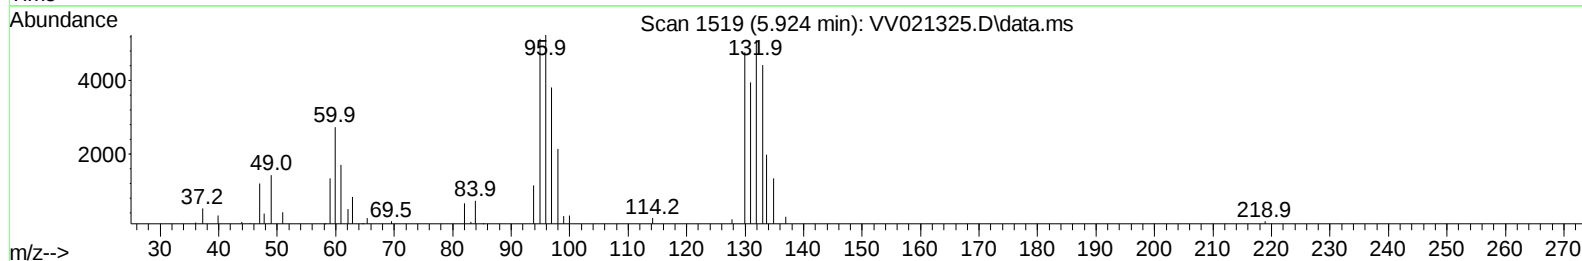


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV050721\  
Data File : VV021325.D  
Acq On : 07 May 2021 14:35  
Operator : SY/MD  
Sample : M2320-03DL 2X  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 10 Sample Multiplier: 1

Quant Time: May 08 00:37:10 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM050321WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat May 08 00:36:06 2021  
Response via : Initial Calibration

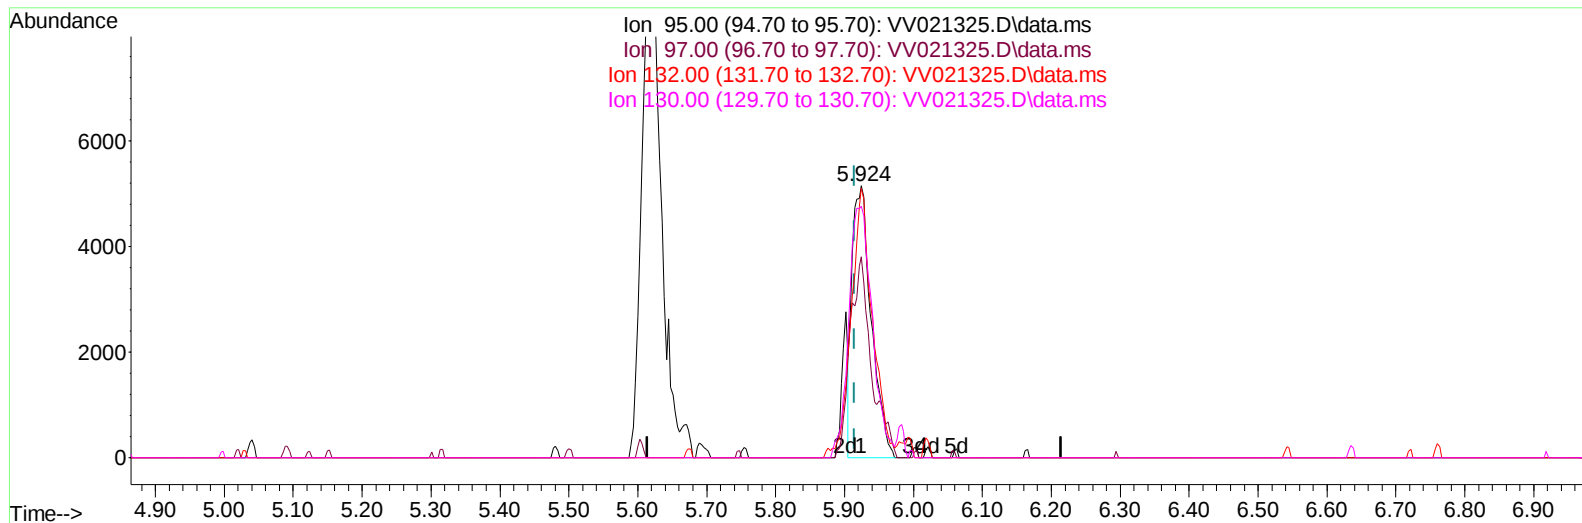

TIC: VV021325.D\data.ms

**(34) Trichloroethene (T)**

5.924min (+ 0.010) 1.99 ug/L

response 9880

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 95.00  | 100.00 | 100.00 |
| 97.00  | 65.00  | 74.02  |
| 132.00 | 101.40 | 99.16  |
| 130.00 | 108.20 | 92.62  |