
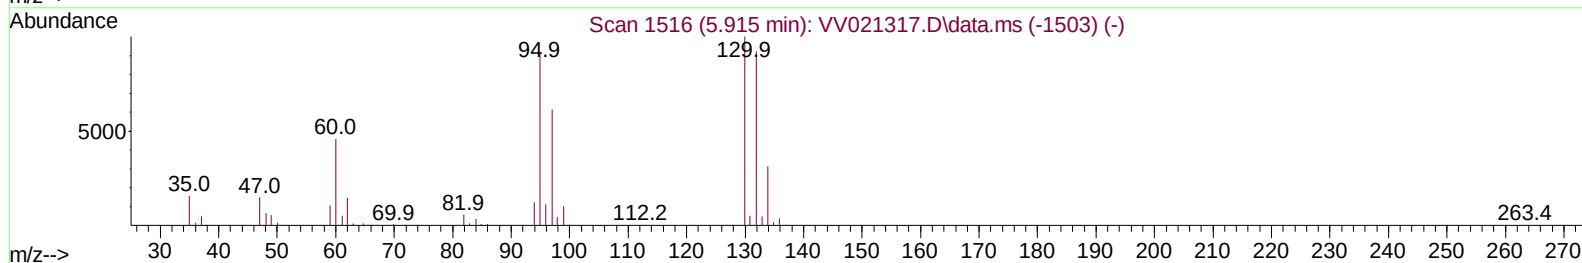
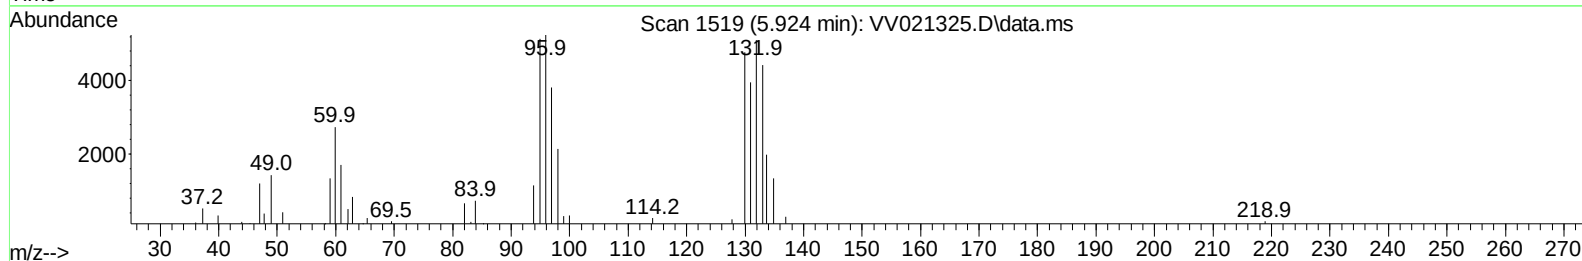


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021325.D
Acq On : 07 May 2021 14:35
Operator : SY/MD
Sample : M2320-03DL 2X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: May 08 00:37:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 08 00:36:06 2021
Response via : Initial Calibration

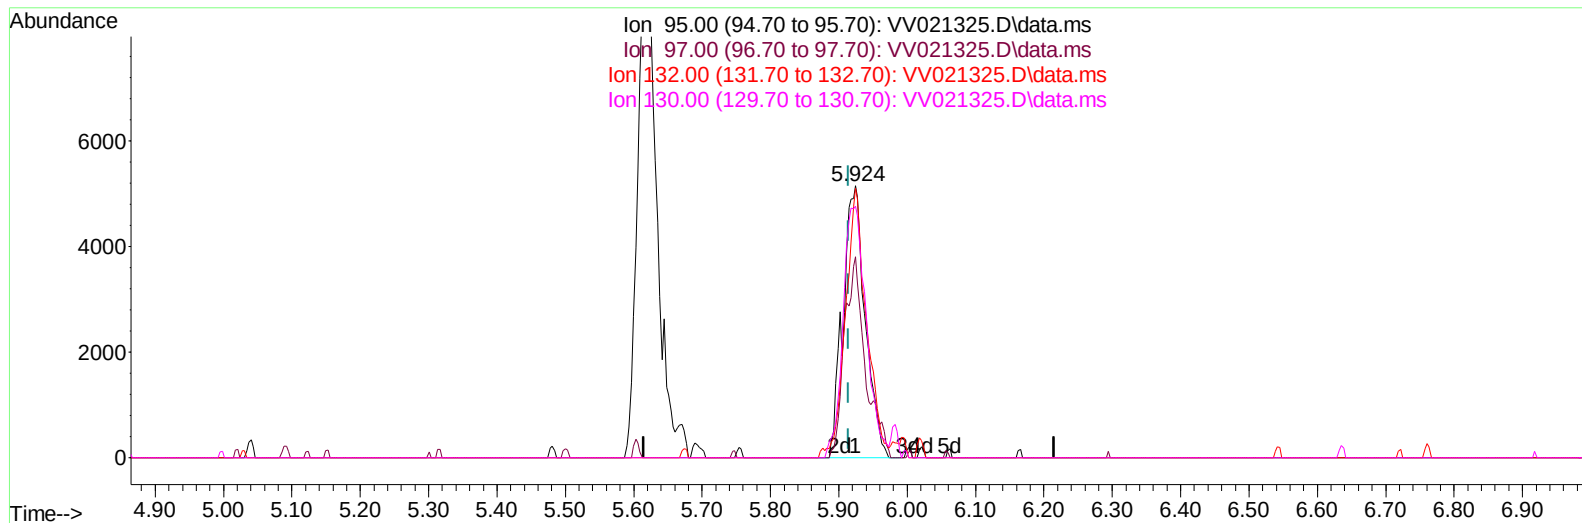

TIC: VV021325.D\data.ms

(34) Trichloroethene (T)

5.924min (+ 0.010) 2.33 ug/L m

response 11603

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	65.00	74.02
132.00	101.40	99.16
130.00	108.20	92.62