
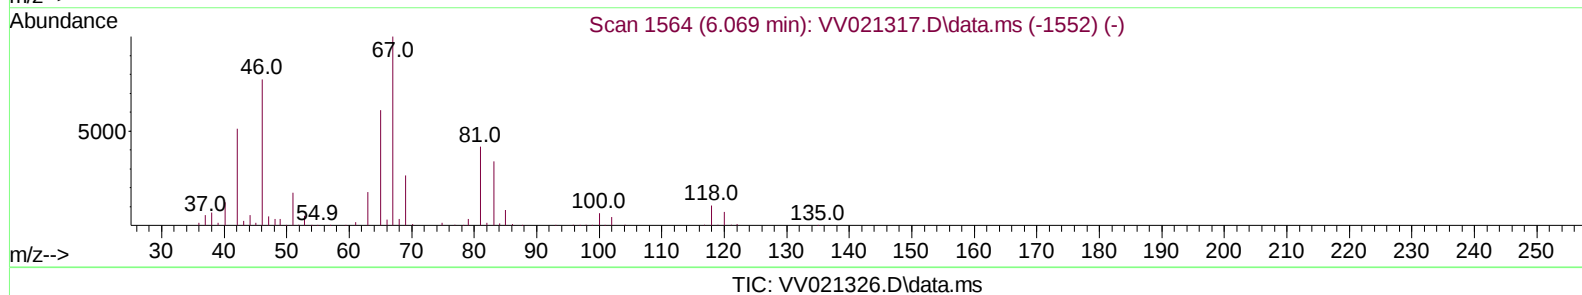
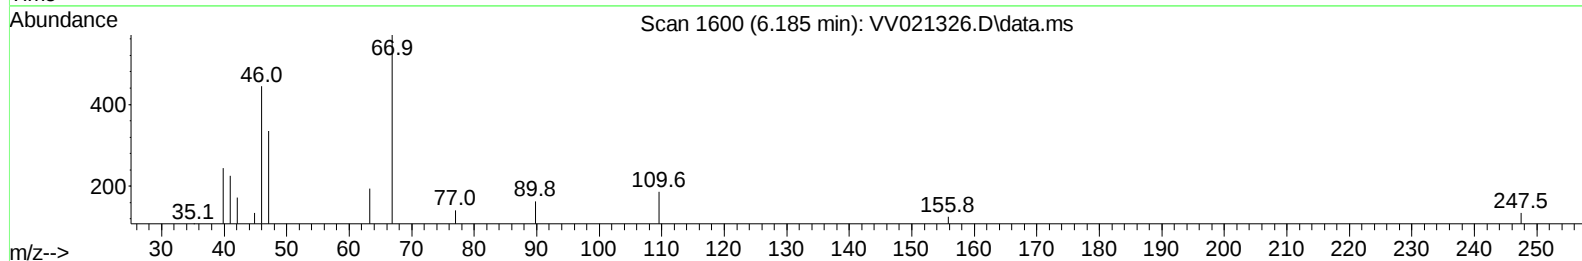


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021326.D
Acq On : 07 May 2021 15:01
Operator : SY/MD
Sample : M2308-01 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: May 08 00:37:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 08 00:36:06 2021
Response via : Initial Calibration

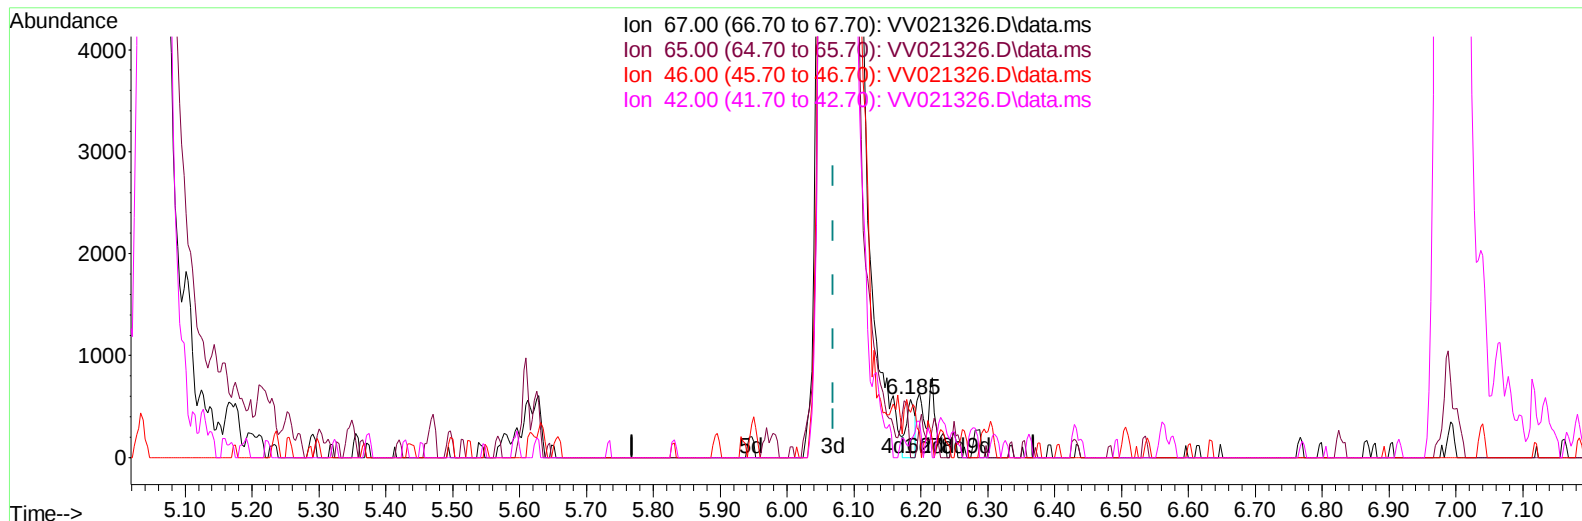

(36) 1,2-Dichloropropane-d6 (S)

6.185min (+ 0.116) 0.13 ug/L

response 488

Ion	Exp%	Act%
67.00	100.00	100.00
65.00	65.10	81.76
46.00	52.60	40.98
42.00	30.80	29.51