
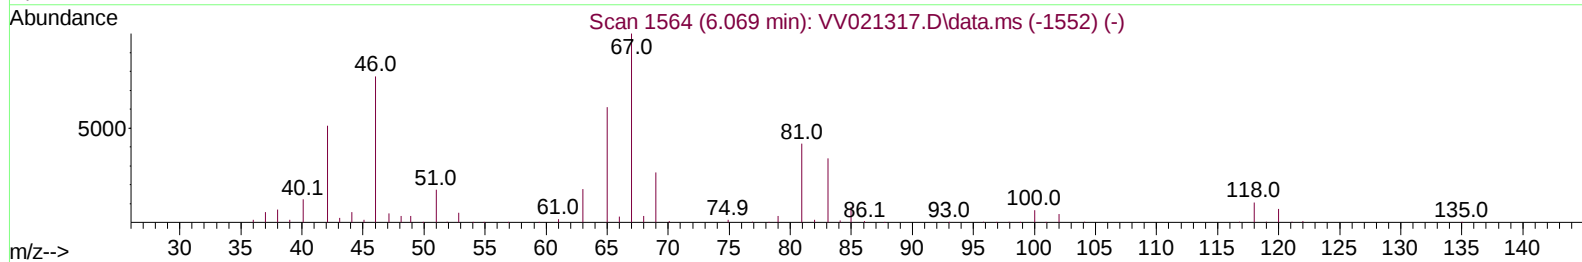
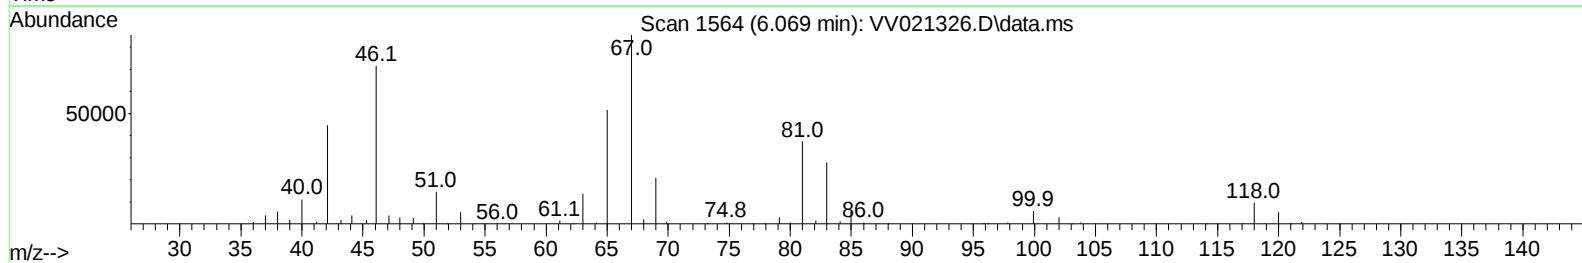


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021326.D
 Acq On : 07 May 2021 15:01
 Operator : SY/MD
 Sample : M2308-01 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: May 08 00:37:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 08 00:36:06 2021
 Response via : Initial Calibration

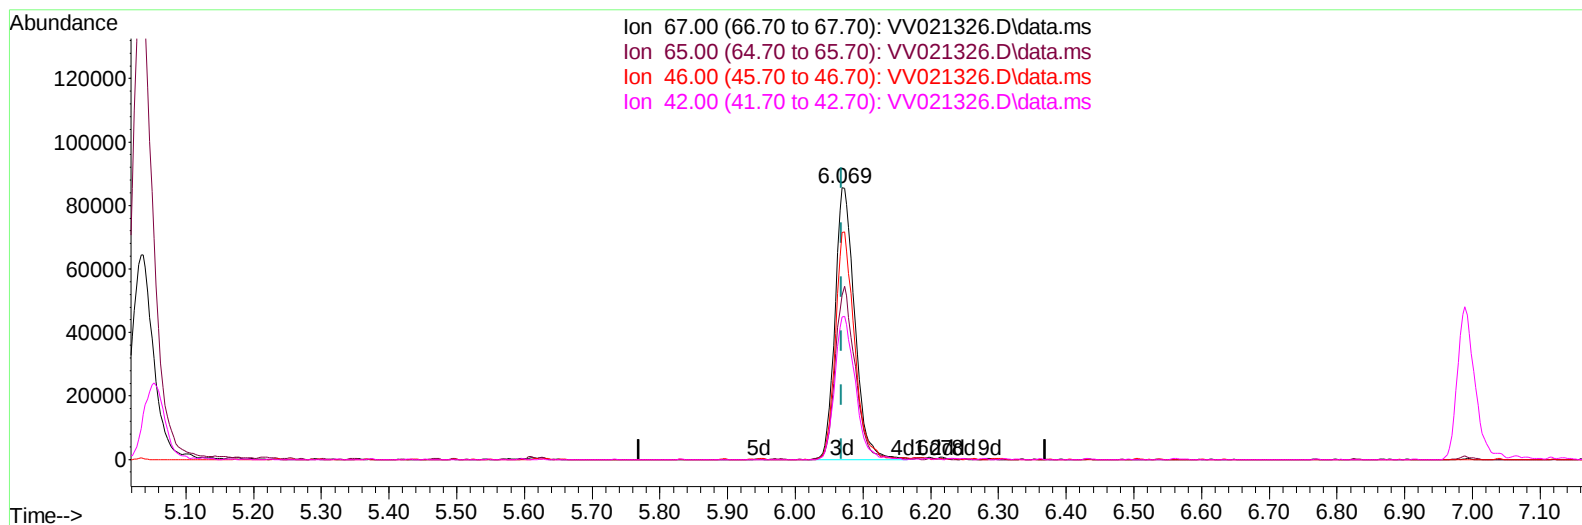

TIC: VV021326.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

6.069min (+ 0.000) 47.80 ug/L m

response 173430

Ion	Exp%	Act%
67.00	100.00	100.00
65.00	65.10	0.23#
46.00	52.60	0.12#
42.00	30.80	0.08#