
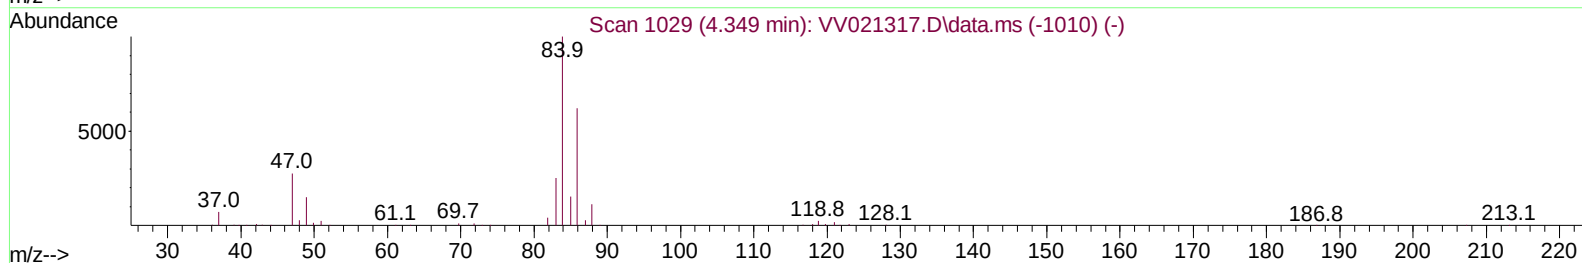
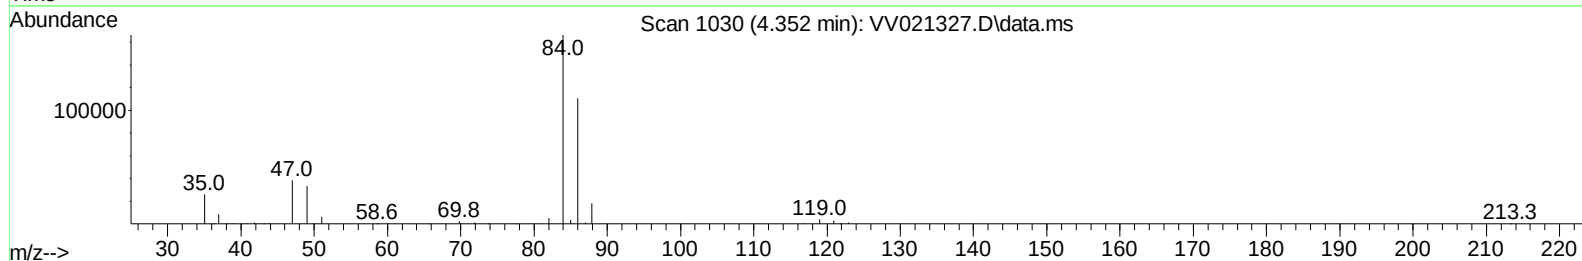


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021327.D
Acq On : 07 May 2021 15:25
Operator : SY/MD
Sample : M2327-03DL 8000X
Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Quant Time: May 08 00:37:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 08 00:36:06 2021
Response via : Initial Calibration

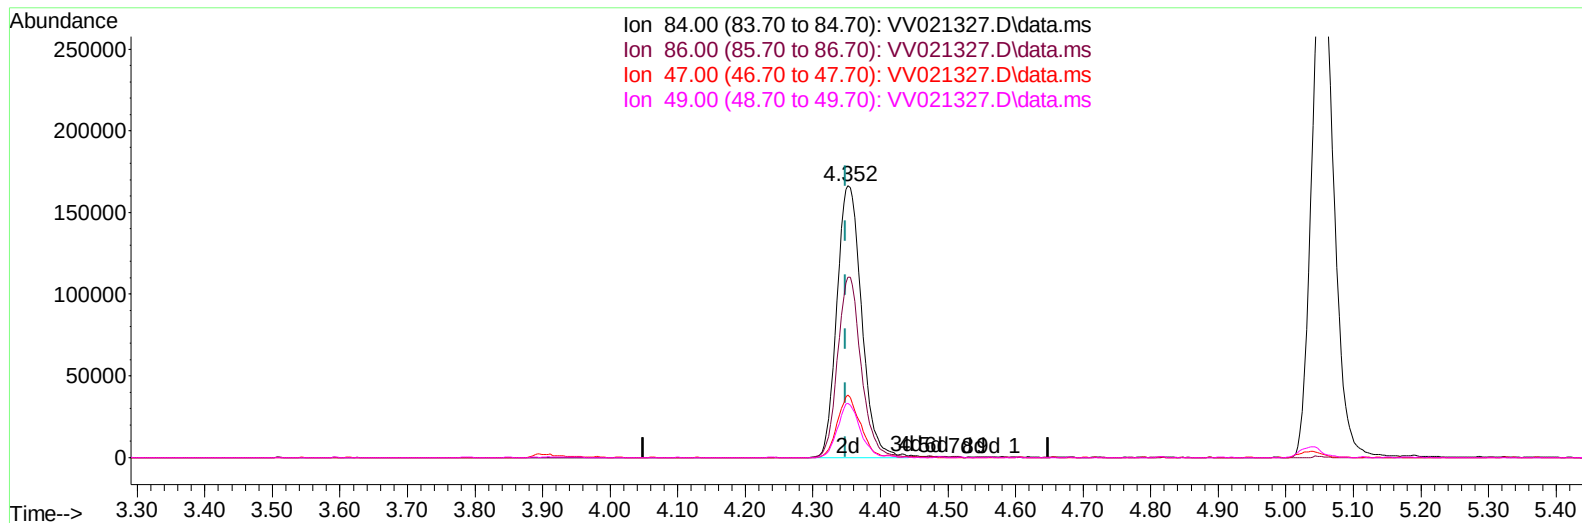

TIC: VV021327.D\data.ms

(24) Chloroform-d (S)

4.352min (+ 0.003) 45.88 ug/L m

response 421637

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.20	0.03#
47.00	38.10	0.02#
49.00	22.10	0.01#