
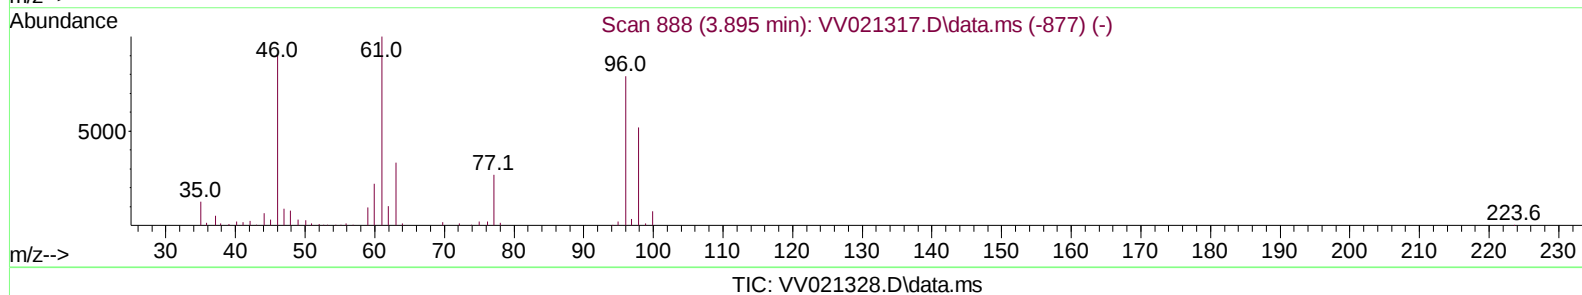
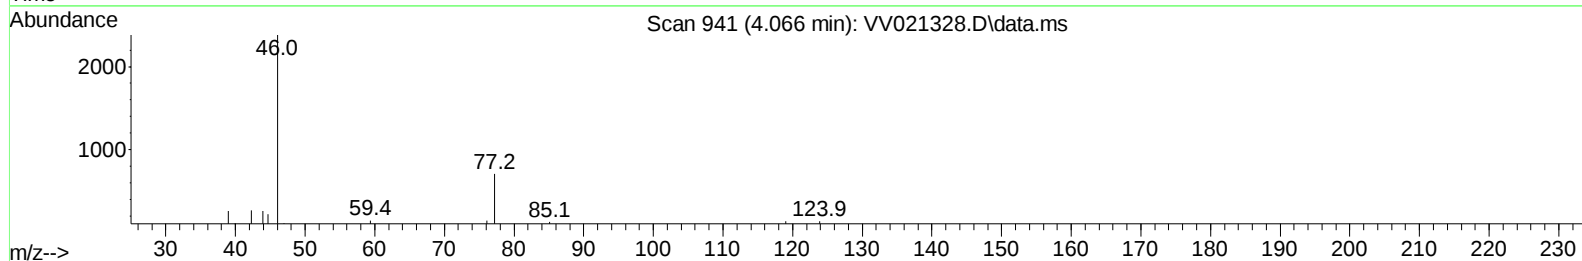


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021328.D
Acq On : 07 May 2021 15:48
Operator : SY/MD
Sample : M2320-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: May 08 00:37:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 08 00:36:06 2021
Response via : Initial Calibration

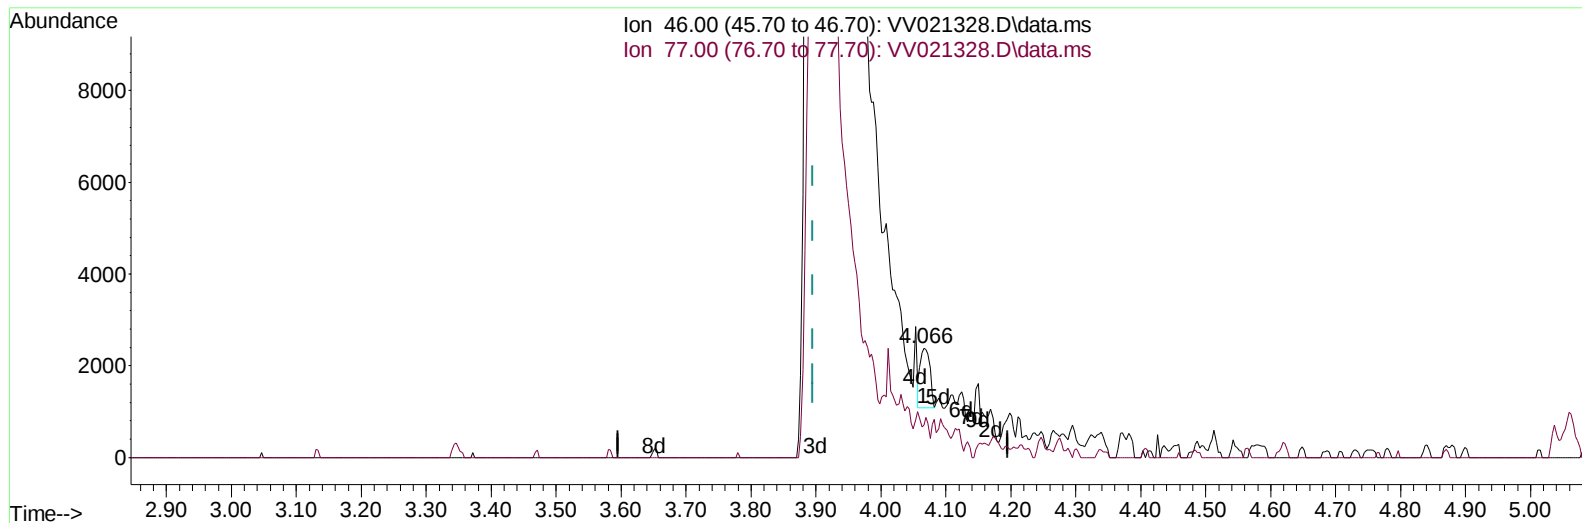

(21) 2-Butanone-d5 (S)

4.066min (+ 0.171) 0.76 ug/L

response 1356

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.60	28.02
0.00	0.00	0.00
0.00	0.00	0.00