
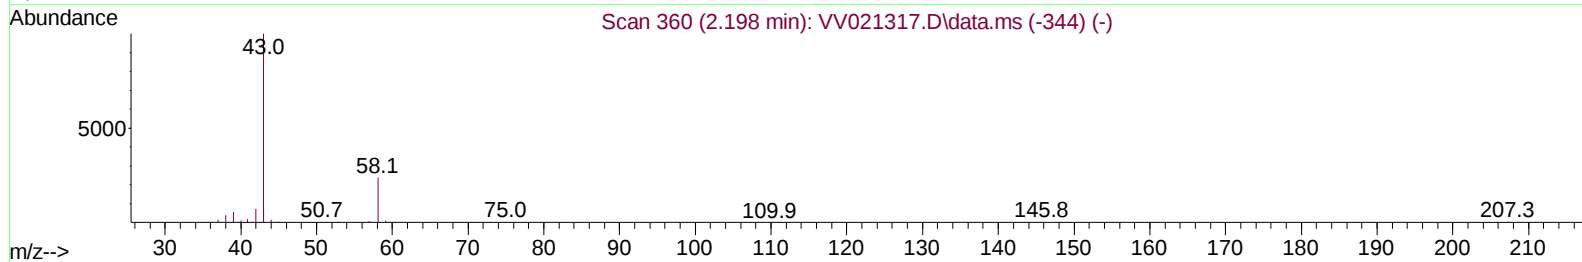
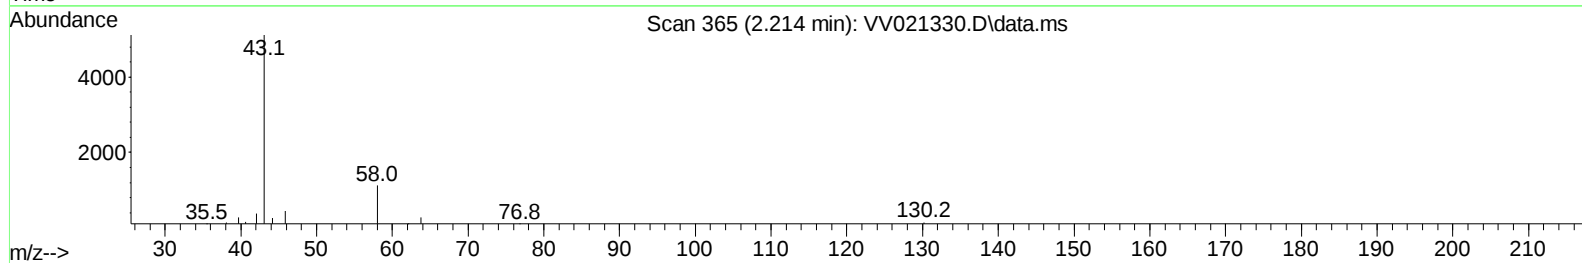


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021330.D
 Acq On : 07 May 2021 16:59
 Operator : SY/MD
 Sample : M2316-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: May 08 00:37:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 08 00:36:06 2021
 Response via : Initial Calibration

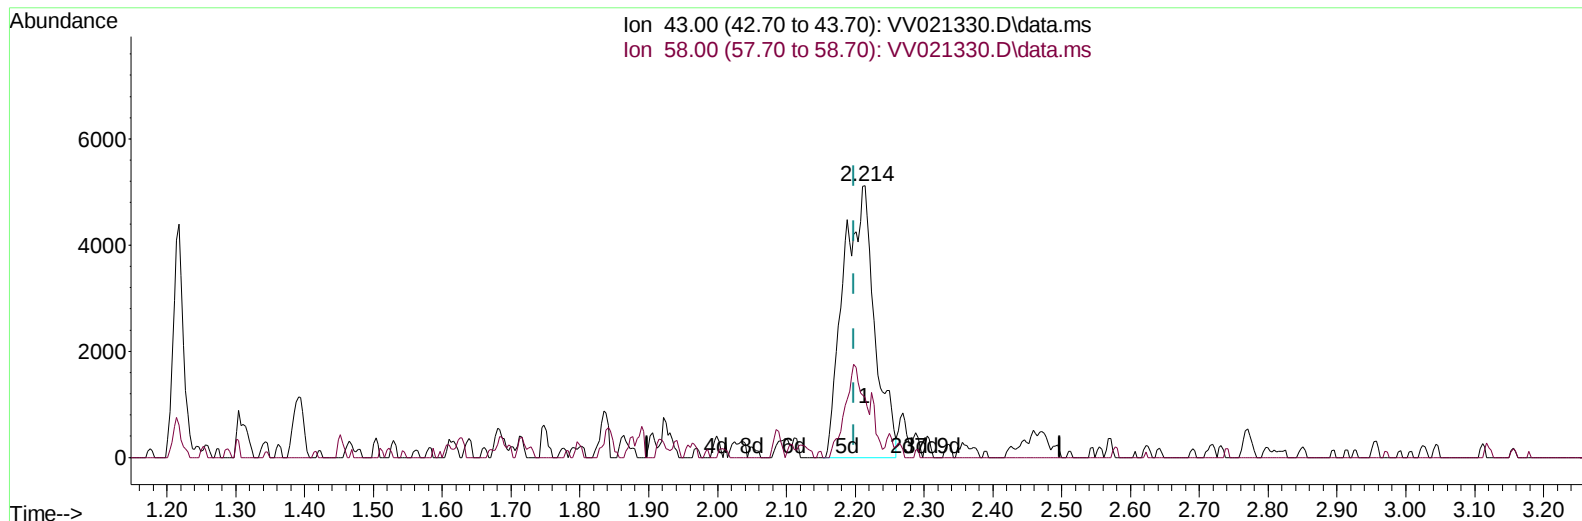

TIC: VV021330.D\data.ms

(13) Acetone (T)

2.214min (+ 0.016) 8.37 ug/L m

response 15994

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	4.21
0.00	0.00	0.00
0.00	0.00	0.00