
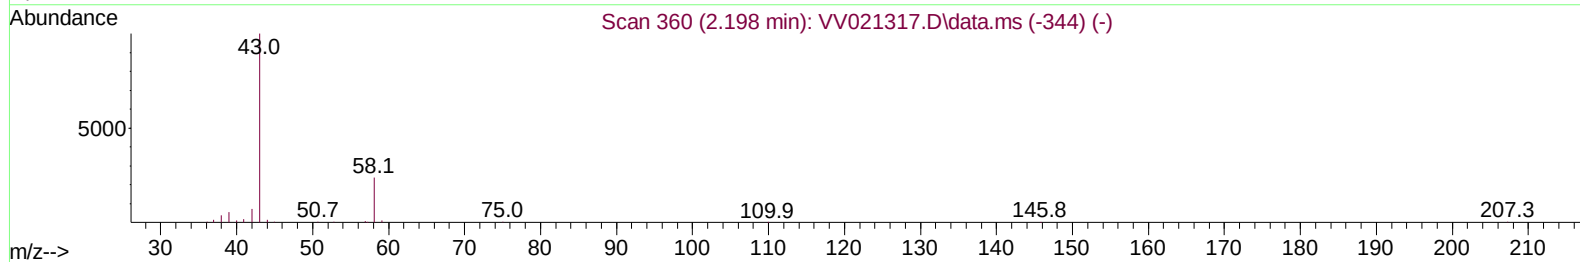
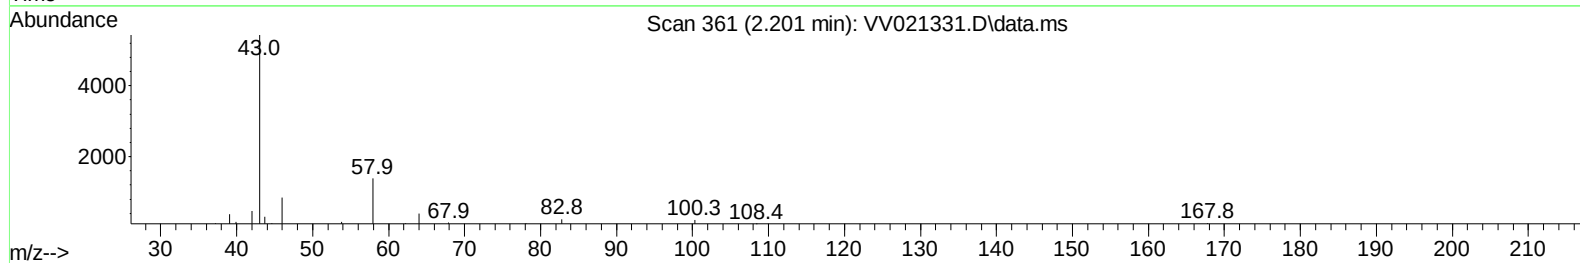


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021331.D
Acq On : 07 May 2021 17:23
Operator : SY/MD
Sample : M2316-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: May 08 00:37:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 08 00:36:06 2021
Response via : Initial Calibration

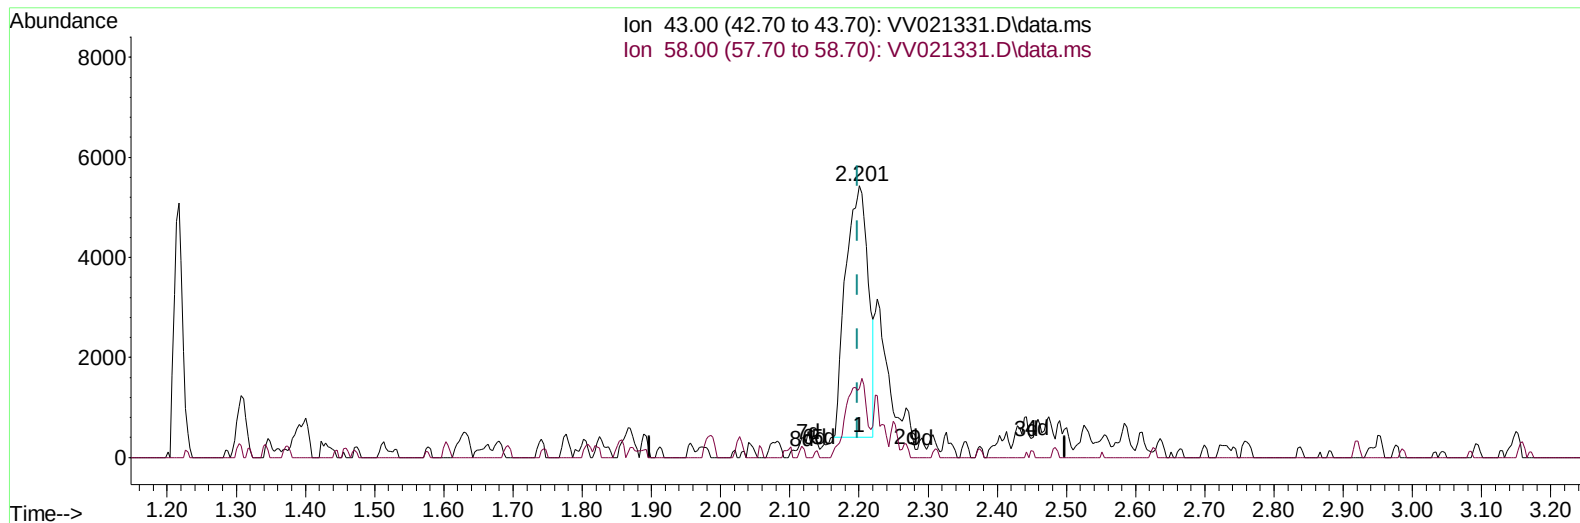

TIC: VV021331.D\data.ms

(13) Acetone (T)

2.201min (+ 0.003) 5.79 ug/L

response 11444

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	11.08
0.00	0.00	0.00
0.00	0.00	0.00