
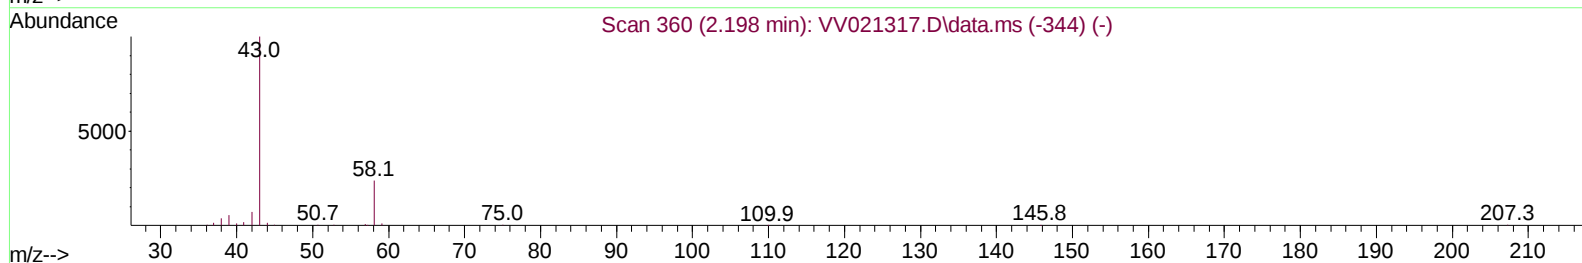
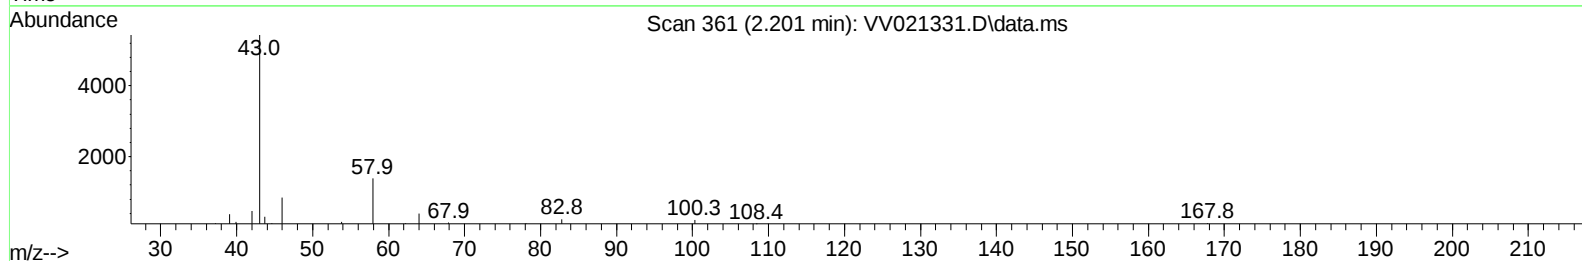


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021331.D
 Acq On : 07 May 2021 17:23
 Operator : SY/MD
 Sample : M2316-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: May 08 00:37:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 08 00:36:06 2021
 Response via : Initial Calibration

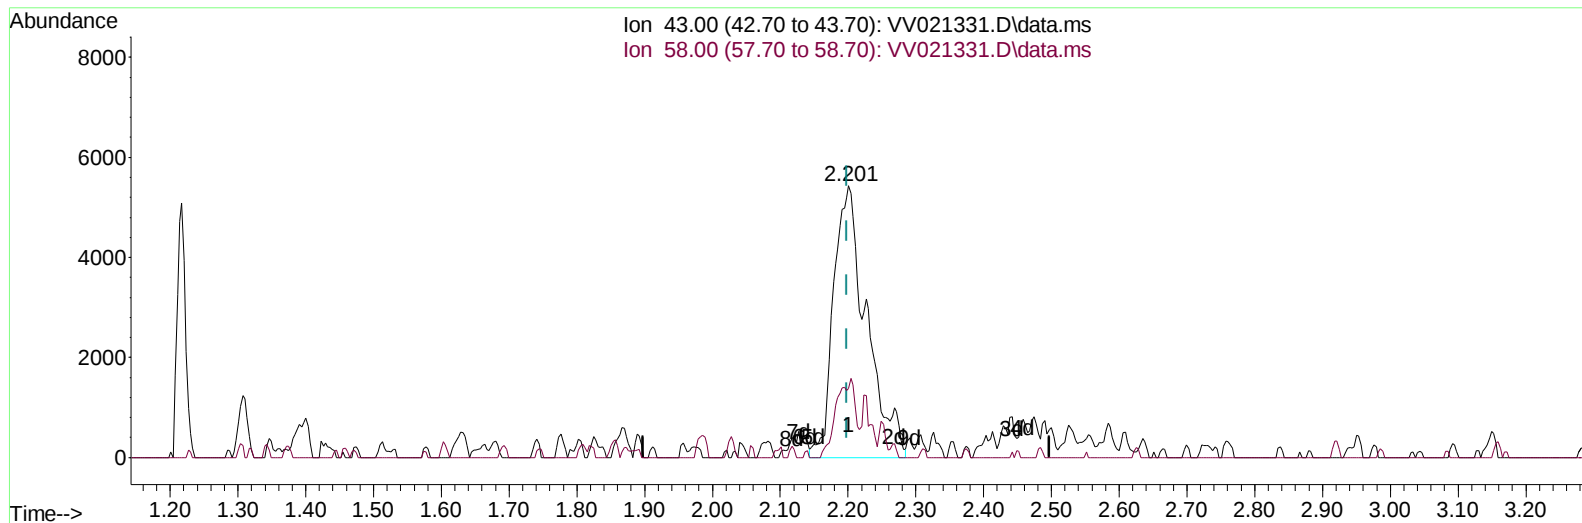

TIC: VV021331.D\data.ms

(13) Acetone (T)

2.201min (+ 0.003) 9.26 ug/L m

response 18299

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	15.40	6.93
0.00	0.00	0.00
0.00	0.00	0.00