
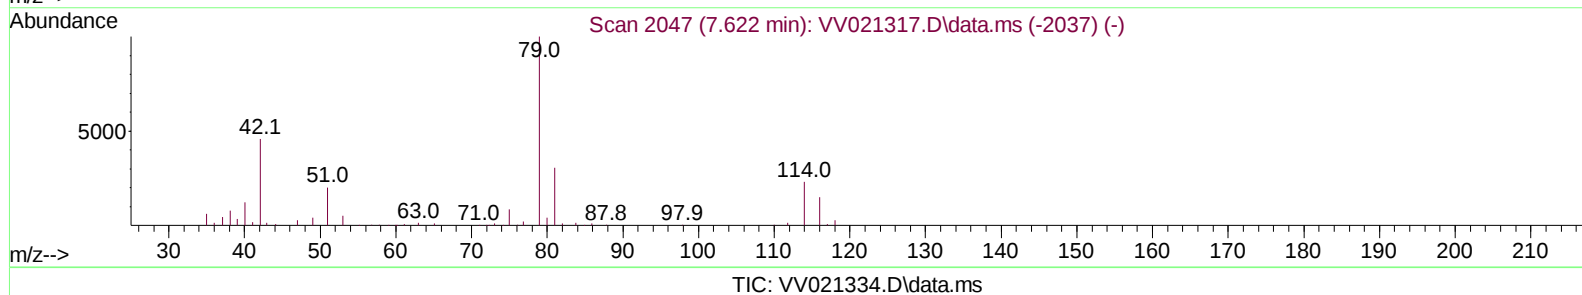
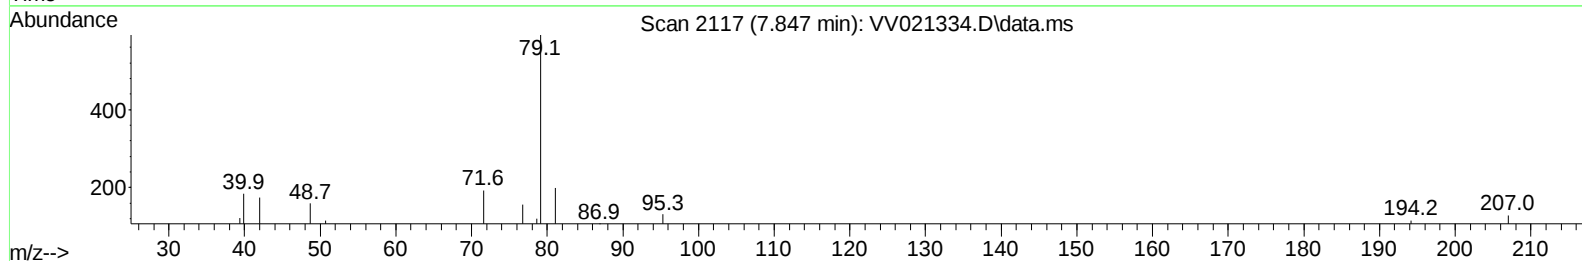


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021334.D
Acq On : 07 May 2021 18:33
Operator : SY/MD
Sample : M2308-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: May 08 00:38:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 08 00:36:06 2021
Response via : Initial Calibration

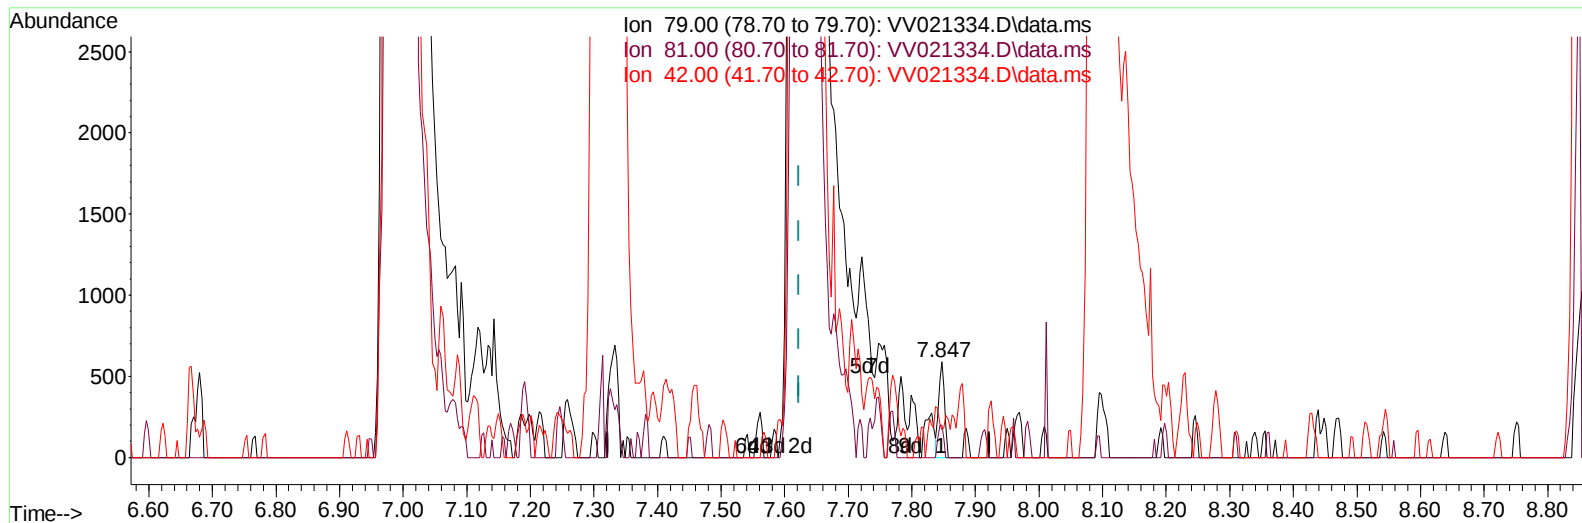

(43) trans-1,3-Dichloropropene-d4 (S)

7.847min (+ 0.225) 0.13 ug/L

response 374

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	32.90	32.09
42.00	35.10	43.85
0.00	0.00	0.00