
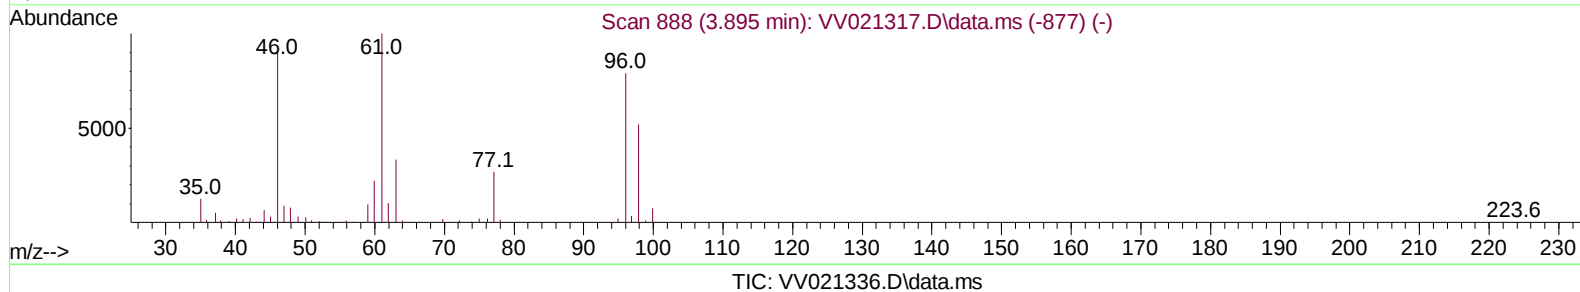
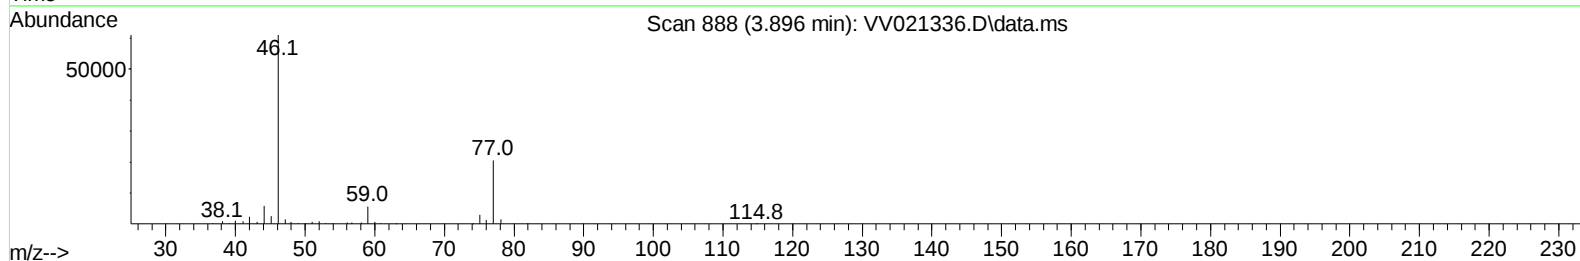


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021336.D
 Acq On : 07 May 2021 19:21
 Operator : SY/MD
 Sample : M2316-03 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 08 00:38:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 08 00:36:06 2021
 Response via : Initial Calibration

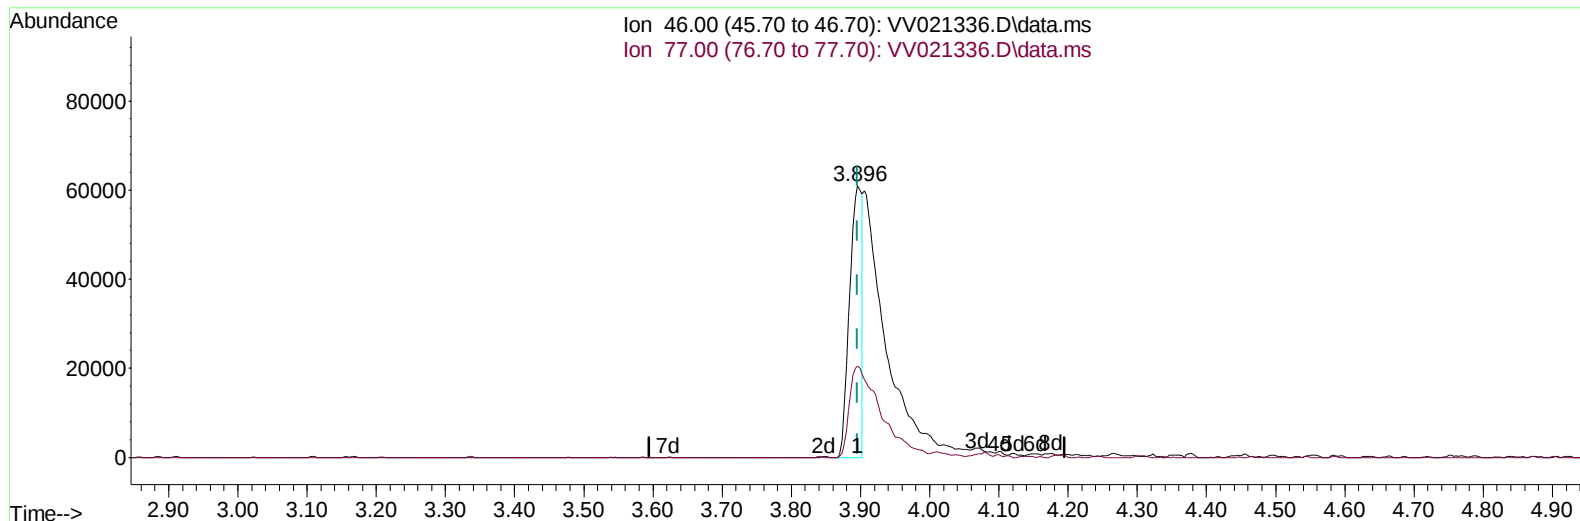

(21) 2-Butanone-d5 (S)

3.896min (+ 0.000) 33.89 ug/L

response 77050

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.60	84.60#
0.00	0.00	0.00
0.00	0.00	0.00