
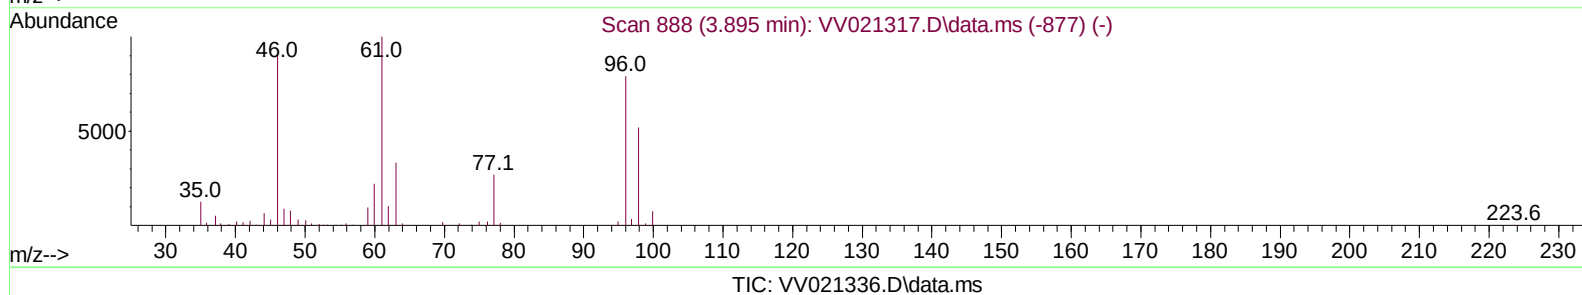
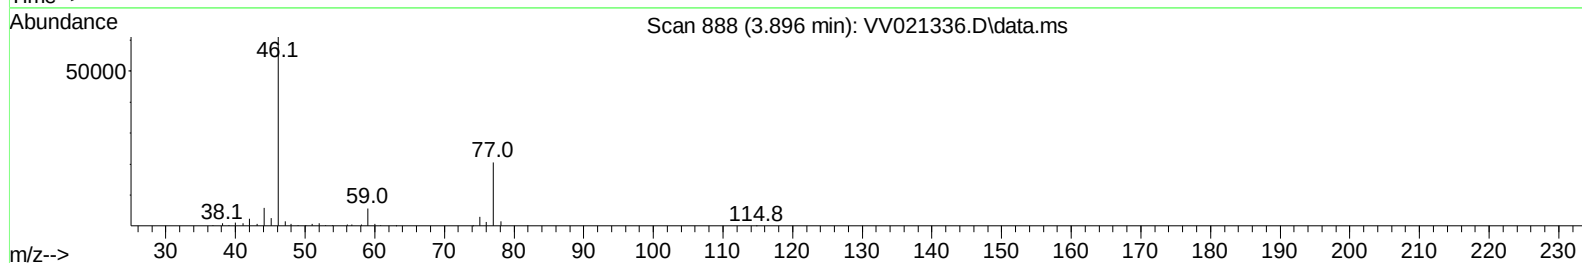


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021336.D
Acq On : 07 May 2021 19:21
Operator : SY/MD
Sample : M2316-03 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 08 00:38:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 08 00:36:06 2021
Response via : Initial Calibration

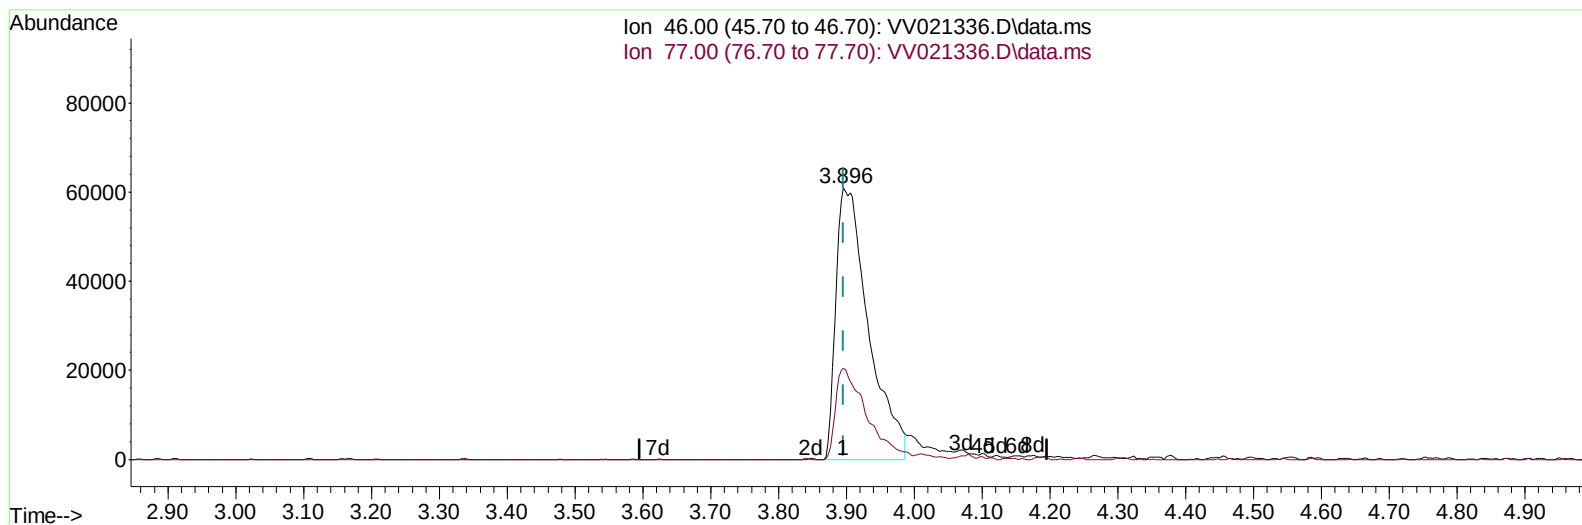

(21) 2-Butanone-d5 (S)

3.896min (+ 0.000) 89.23 ug/L m

response 202860

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.60	32.13
0.00	0.00	0.00
0.00	0.00	0.00