

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021325.D
 Acq On : 07 May 2021 14:35
 Operator : SY/MD
 Sample : M2320-03DL 2X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3A07DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M

Title : VOC Analysis

Signal : TIC: VV021325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rBV	263241	260112	10.68%	1.248%
2	1.571	158	165	175	rVB	220314	248454	10.20%	1.192%
3	2.108	323	332	346	rBV	539203	780611	32.05%	3.745%
4	2.326	396	400	402	rBV4	1964	1614	0.07%	0.008%
5	2.407	416	425	427	rBV6	1249	1824	0.07%	0.009%
6	2.510	448	457	469	rVB7	10311	16025	0.66%	0.077%
7	2.561	469	473	475	rBV4	2043	1666	0.07%	0.008%
8	2.683	507	511	516	rBV8	2174	2079	0.09%	0.010%
9	2.770	522	538	566	rBV	1149536	2435692	100.00%	11.685%
10	3.066	628	630	633	rVB3	2253	1120	0.05%	0.005%
11	3.101	638	641	644	rBV2	1288	934	0.04%	0.004%
12	3.166	653	661	668	rBV10	920	1534	0.06%	0.007%
13	3.195	668	670	673	rVB2	1451	791	0.03%	0.004%
14	3.272	689	694	698	rBV5	1242	1081	0.04%	0.005%
15	3.407	733	736	740	rVB3	1284	904	0.04%	0.004%
16	3.587	789	792	798	rBV5	1438	1112	0.05%	0.005%
17	3.616	798	801	803	rBV3	1278	785	0.03%	0.004%
18	3.661	813	815	820	rVB3	1102	820	0.03%	0.004%
19	3.716	827	832	834	rBV5	1159	1109	0.05%	0.005%
20	3.831	863	868	872	rBV5	1476	1539	0.06%	0.007%
21	3.902	877	890	922	rBV	108441	392606	16.12%	1.883%
22	4.207	981	985	991	rBV7	1717	2170	0.09%	0.010%
23	4.240	992	995	998	rBV5	1423	837	0.03%	0.004%
24	4.349	1015	1029	1050	rBV	429727	1036738	42.56%	4.973%
25	4.603	1103	1108	1109	rBV5	1277	1216	0.05%	0.006%
26	4.638	1115	1119	1122	rBV4	1184	1046	0.04%	0.005%
27	4.683	1129	1133	1138	rBV5	1446	1250	0.05%	0.006%
28	4.799	1166	1169	1172	rBV4	2003	1367	0.06%	0.007%
29	4.851	1179	1185	1186	rBV4	1894	1703	0.07%	0.008%
30	5.047	1226	1246	1270	rBV2	900865	2323340	95.39%	11.146%
31	5.442	1363	1369	1372	rBV7	1971	1762	0.07%	0.008%
32	5.619	1412	1424	1444	rBV	745995	1503261	61.72%	7.212%
33	5.915	1502	1516	1535	rBV6	67157	162523	6.67%	0.780%
34	6.072	1551	1565	1588	rBV2	488647	995947	40.89%	4.778%
35	6.510	1699	1701	1706	rVB4	1155	1030	0.04%	0.005%
36	6.535	1706	1709	1713	rBV3	1422	1019	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021325.D
 Acq On : 07 May 2021 14:35
 Operator : SY/MD
 Sample : M2320-03DL 2X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3A07DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis

37	6.587	1721	1725	1727	rBV4	1258	906	0.04%	0.004%
38	6.638	1738	1741	1745	rVB6	1895	1160	0.05%	0.006%
39	6.712	1757	1764	1770	rVB8	1442	1454	0.06%	0.007%
40	6.834	1799	1802	1806	rBV3	1301	954	0.04%	0.005%
41	6.883	1812	1817	1820	rBV5	1626	1547	0.06%	0.007%
42	6.934	1830	1833	1837	rBV3	1387	958	0.04%	0.005%
43	6.989	1837	1850	1872	rBV	310479	565193	23.20%	2.711%
44	7.320	1941	1953	1972	rBV	1109946	1925949	79.07%	9.239%
45	7.625	2038	2048	2064	rBV	227875	396079	16.26%	1.900%
46	7.841	2112	2115	2116	rBV2	2033	1103	0.05%	0.005%
47	7.889	2125	2130	2133	rBV4	2021	1946	0.08%	0.009%
48	7.982	2148	2159	2172	rVV4	104038	180448	7.41%	0.866%
49	8.095	2184	2194	2227	rBV2	447689	895684	36.77%	4.297%
50	8.352	2271	2274	2277	rVB3	2893	1820	0.07%	0.009%
51	8.384	2277	2284	2287	rBV8	2157	2472	0.10%	0.012%
52	8.445	2300	2303	2306	rBV3	3073	2078	0.09%	0.010%
53	8.857	2417	2431	2451	rBV	1138778	1847979	75.87%	8.865%
54	9.082	2498	2501	2503	rVB3	1841	1008	0.04%	0.005%
55	9.130	2513	2516	2518	rBV3	1893	1240	0.05%	0.006%
56	9.391	2593	2597	2599	rBV2	974	832	0.03%	0.004%
57	9.509	2627	2634	2638	rVB5	1240	1474	0.06%	0.007%
58	9.715	2696	2698	2702	rBV2	1020	844	0.03%	0.004%
59	9.792	2719	2722	2727	rVB5	1754	1194	0.05%	0.006%
60	9.828	2727	2733	2738	rVB6	2055	2347	0.10%	0.011%
61	9.873	2744	2747	2750	rBV4	1896	1576	0.06%	0.008%
62	9.947	2767	2770	2775	rVB4	2153	1843	0.08%	0.009%
63	9.979	2775	2780	2782	rBV2	1702	1423	0.06%	0.007%
64	10.220	2843	2855	2881	rBV	685576	1088607	44.69%	5.222%
65	10.426	2917	2919	2923	rVB	1390	859	0.04%	0.004%
66	10.458	2923	2929	2932	rBV6	2632	2425	0.10%	0.012%
67	10.677	2995	2997	3001	rVV4	1389	816	0.03%	0.004%
68	10.754	3018	3021	3024	rVB3	1416	1081	0.04%	0.005%
69	10.776	3024	3028	3032	rBV3	2584	1681	0.07%	0.008%
70	10.853	3050	3052	3057	rVB3	1556	1127	0.05%	0.005%
71	10.921	3065	3073	3075	rBV6	5899	6394	0.26%	0.031%
72	11.027	3102	3106	3109	rBV3	1590	1349	0.06%	0.006%
73	11.149	3140	3144	3149	rVB5	3439	3383	0.14%	0.016%
74	11.255	3164	3177	3201	rBV	1156663	1795968	73.74%	8.616%
75	11.497	3243	3252	3255	rVB9	1865	2620	0.11%	0.013%
76	11.632	3281	3294	3310	rBV	1204286	1877524	77.08%	9.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021325.D
 Acq On : 07 May 2021 14:35
 Operator : SY/MD
 Sample : M2320-03DL 2X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3A07DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M

Title : VOC Analysis

77	11.837	3354	3358	3361	rBV4	1890	1630	0.07%	0.008%
78	11.947	3390	3392	3394	rBV3	1684	825	0.03%	0.004%
79	12.040	3419	3421	3424	rBV2	1805	1121	0.05%	0.005%
80	12.188	3463	3467	3470	rBV3	1759	1511	0.06%	0.007%
81	12.342	3513	3515	3518	rBV4	1196	852	0.03%	0.004%
82	12.358	3518	3520	3523	rVV3	1468	1019	0.04%	0.005%
83	12.484	3552	3559	3563	rBV7	2532	3223	0.13%	0.015%
84	12.580	3586	3589	3592	rVB4	1731	1142	0.05%	0.005%
85	12.599	3592	3595	3598	rBV4	1569	1256	0.05%	0.006%
86	12.699	3619	3626	3630	rBV8	1728	2174	0.09%	0.010%
87	12.744	3637	3640	3642	rBV2	1312	848	0.03%	0.004%
88	12.799	3655	3657	3660	rBV2	1595	1050	0.04%	0.005%
89	13.001	3717	3720	3723	rBV4	1466	890	0.04%	0.004%
90	13.146	3763	3765	3768	rBV2	1711	1012	0.04%	0.005%
91	13.320	3816	3819	3822	rBV5	1397	1310	0.05%	0.006%
92	13.529	3881	3884	3887	rBV5	1830	1439	0.06%	0.007%
93	13.686	3931	3933	3938	rBV3	1321	1326	0.05%	0.006%
94	13.921	4002	4006	4007	rBV4	1389	808	0.03%	0.004%
95	13.953	4014	4016	4020	rBV4	1248	1042	0.04%	0.005%
96	14.284	4116	4119	4122	rBV5	1456	977	0.04%	0.005%
97	14.307	4122	4126	4129	rBV5	1719	1593	0.07%	0.008%
98	14.493	4181	4184	4188	rBV5	3239	1920	0.08%	0.009%
99	14.516	4188	4191	4193	rBV4	3411	1845	0.08%	0.009%
100	15.230	4410	4413	4415	rBV4	2283	1487	0.06%	0.007%




Sum of corrected areas: 20845266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021325.D
Acq On : 07 May 2021 14:35
Operator : SY/MD
Sample : M2320-03DL 2X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3A07DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

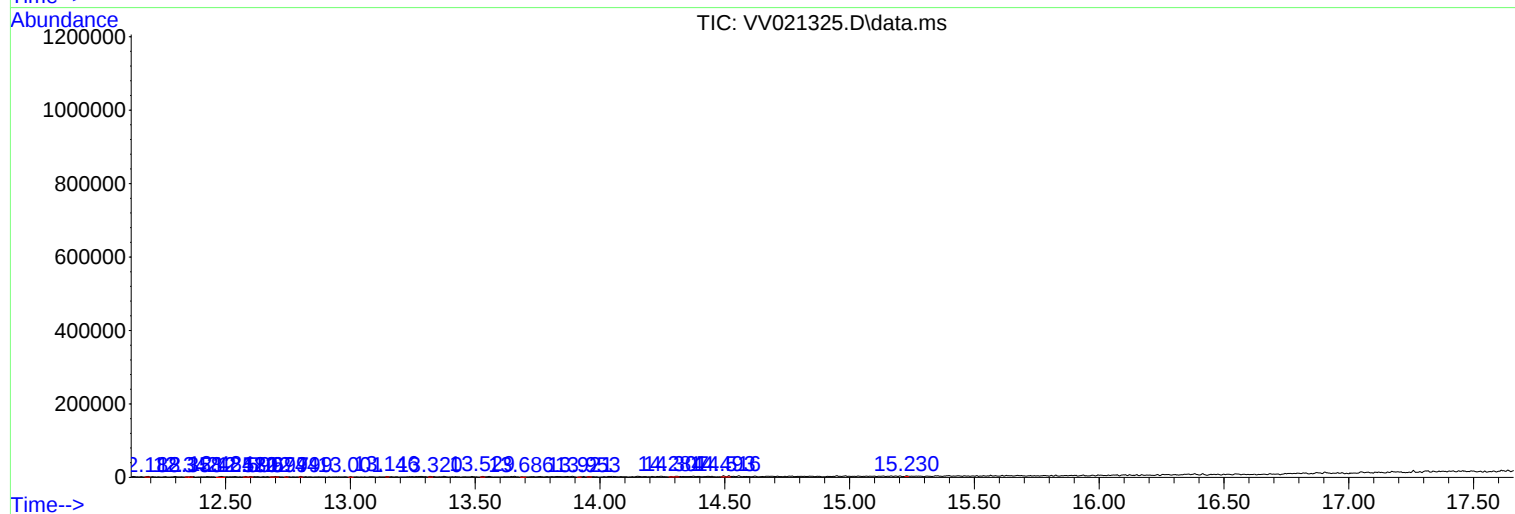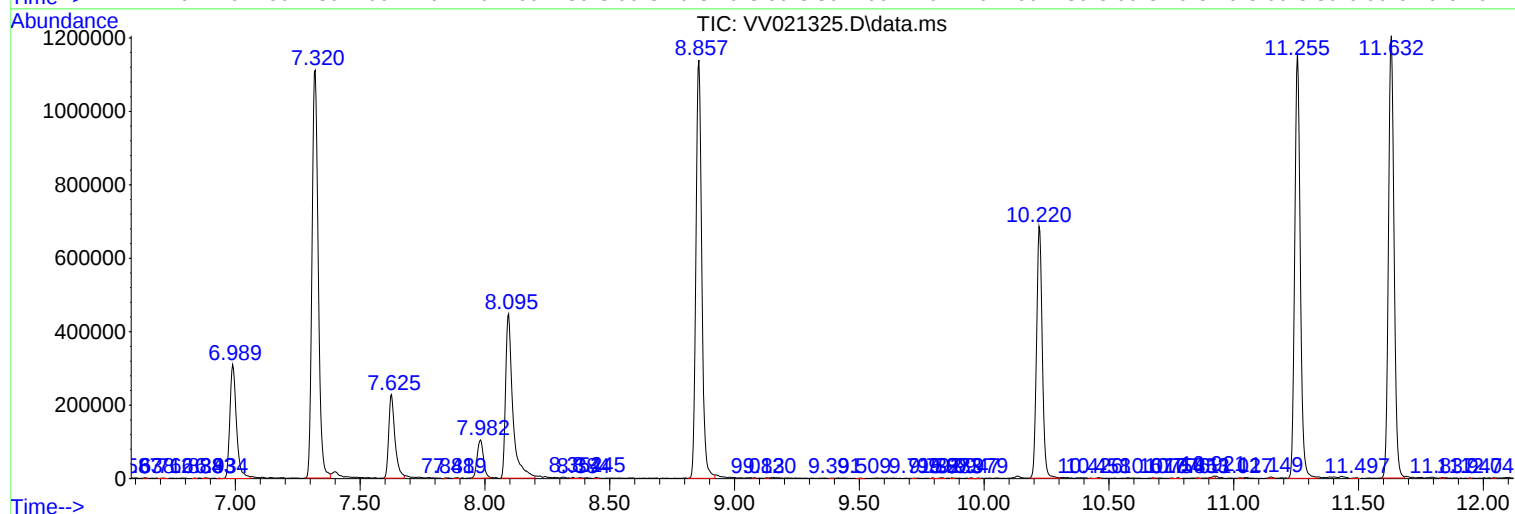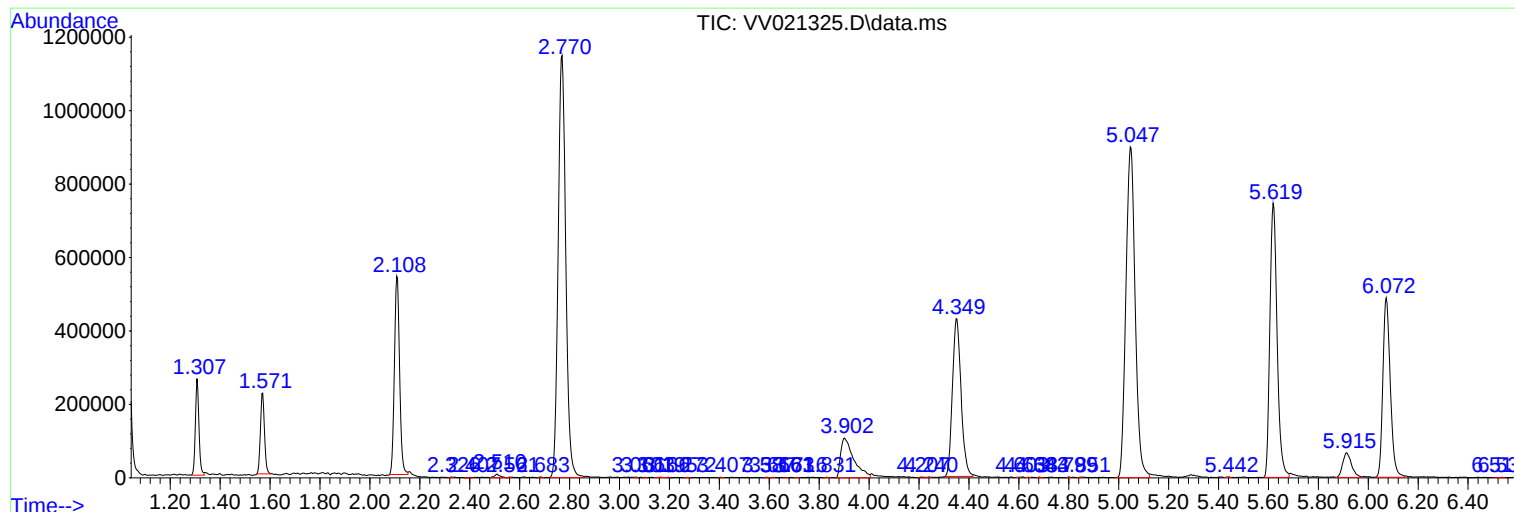

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021325.D
Acq On : 07 May 2021 14:35
Operator : SY/MD
Sample : M2320-03DL 2X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3A07DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
Data File : VV021325.D
Acq On : 07 May 2021 14:35
Operator : SY/MD
Sample : M2320-03DL 2X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3A07DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
