
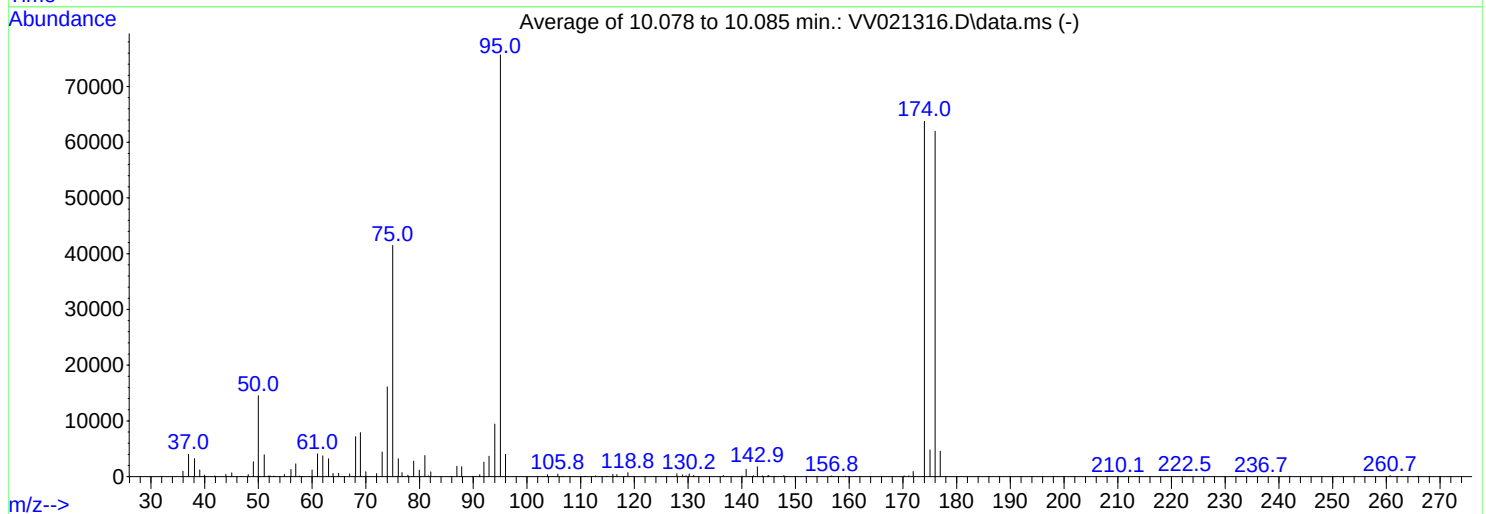


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050721\
 Data File : VV021316.D
 Acq On : 07 May 2021 10:03
 Operator : SY/MD
 Sample : BFB97
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB197

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050321WMA.M
 Title : VOC Analysis
 Last Update : Sat May 08 00:36:06 2021

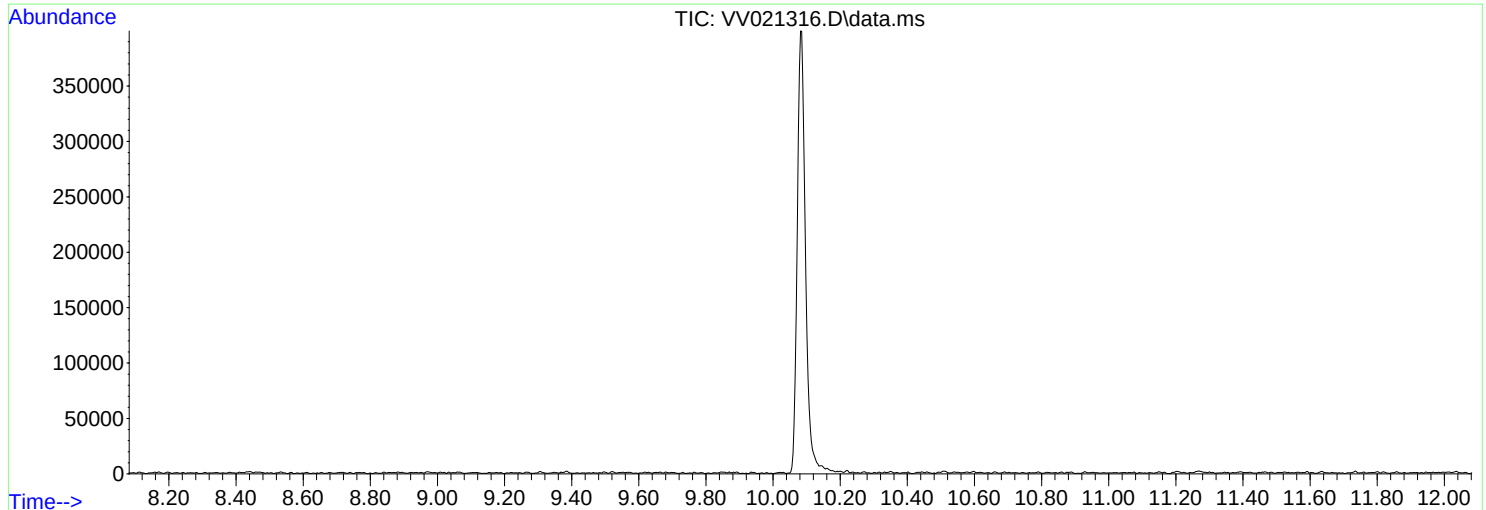

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	14539	PASS
75	95	30	80	54.8	41475	PASS
95	95	100	100	100.0	75677	PASS
96	95	5	9	5.3	4006	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.3	63773	PASS
175	174	5	9	7.5	4794	PASS
176	174	95	105	97.2	61995	PASS
177	176	5	10	7.4	4576	PASS

m/z	Abundance
35.90	938.0
37.00	4111.0
38.10	3480.0
39.10	1184.0
39.90	261.0
41.90	186.0
44.00	617.0
45.00	751.0
46.80	105.0
48.10	524.0
49.10	2618.0
50.00	15205.0
51.10	3687.0
52.00	292.0
52.90	169.0
54.80	376.0
56.10	1412.0
56.90	2294.0
57.70	123.0
58.20	103.0
60.00	1337.0
61.00	4158.0
62.00	4000.0
63.10	3274.0
63.90	610.0
64.90	618.0
67.00	531.0
68.10	7205.0
69.00	8082.0
70.00	964.0
72.00	551.0
73.00	4605.0
74.00	16704.0
75.00	42664.0
76.00	3157.0
76.80	755.0
77.80	318.0
78.90	2865.0
79.90	1194.0
81.00	3972.0
82.10	898.0
87.00	1867.0
87.80	1702.0
89.80	101.0
91.20	335.0
92.00	2619.0
92.90	3782.0
94.00	9887.0
95.00	78088.0
96.00	4090.0
103.80	326.0
105.80	488.0
106.60	106.0
112.70	119.0
116.00	513.0
116.70	360.0
118.80	706.0
127.90	528.0
129.00	319.0
129.60	152.0
130.20	506.0
131.10	234.0
136.50	195.0
140.80	1487.0
142.20	240.0
142.90	1870.0
143.80	155.0
145.00	374.0
146.10	105.0
147.90	233.0
156.80	181.0
159.30	133.0
170.20	172.0
171.10	190.0
171.90	957.0
174.00	65864.0
175.10	4949.0
176.00	63536.0
176.90	4903.0
260.70	269.0
265.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197

m/z	Abundance
36.00	1078.0
37.00	4110.0
38.10	2856.0
39.10	1181.0
39.90	249.0
41.90	255.0
44.00	706.0
45.10	652.0
48.10	563.0
49.10	2973.0
50.00	14287.0
51.10	3461.0
51.90	269.0
54.80	397.0
56.10	1154.0
56.90	2382.0
60.00	1271.0
61.00	4354.0
62.00	3295.0
63.00	3054.0
64.00	376.0
64.90	411.0
66.00	155.0
67.00	452.0
68.10	6615.0
69.00	7607.0
70.00	848.0
72.00	569.0
73.10	3744.0
74.00	14298.0
75.00	39920.0
76.00	3348.0
76.80	718.0
77.90	197.0
78.90	2844.0
80.00	816.0
81.00	3215.0
82.10	903.0
82.90	124.0
86.90	1509.0
87.90	1985.0
91.10	134.0
92.00	2660.0
93.00	3735.0
94.00	8637.0
95.10	71576.0
96.00	3783.0
103.80	445.0
105.80	523.0
106.70	102.0
112.70	173.0
114.80	133.0
116.00	356.0
116.80	452.0
118.70	767.0
127.90	504.0
129.00	358.0
129.60	142.0
130.20	169.0
131.10	163.0
136.60	400.0
140.00	107.0
140.80	1273.0
142.10	313.0
142.90	1457.0
143.90	146.0
144.80	366.0
147.80	184.0
156.50	143.0
156.70	131.0
159.30	128.0
171.10	134.0
172.00	969.0
174.00	59416.0
175.00	4683.0
176.00	56408.0
177.00	4376.0
210.10	135.0
222.50	191.0
236.70	126.0
260.70	162.0
265.90	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197

m/z	Abundance
43.80	164.0
48.60	149.0
87.30	170.0
88.10	113.0
274.90	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197

m/z	Abundance
35.90	876.0
37.00	3780.0
38.10	3424.0
39.10	1266.0
40.00	334.0
43.90	419.0
45.00	676.0
49.00	2421.0
50.00	14124.0
51.10	4627.0
52.20	358.0
52.90	177.0
54.90	319.0
56.00	1320.0
57.00	2180.0
57.70	216.0
58.30	104.0
60.00	1007.0
61.00	3696.0
62.00	3910.0
63.10	3312.0
63.80	715.0
65.00	787.0
67.00	523.0
68.10	7712.0
69.00	7989.0
70.00	832.0
72.00	563.0
73.10	4953.0
74.00	17296.0
75.00	41840.0
76.10	3117.0
76.70	672.0
77.80	318.0
78.90	2641.0
79.90	1535.0
81.00	4231.0
81.70	450.0
82.10	794.0
85.80	128.0
86.90	2196.0
87.90	1663.0
89.80	113.0
91.20	590.0
92.00	2538.0
93.00	3527.0
94.00	9843.0
95.00	77368.0
96.00	4145.0
103.80	256.0
104.90	149.0
105.70	396.0
110.80	151.0
112.80	170.0
116.00	426.0
116.70	296.0
118.20	135.0
118.90	664.0
127.90	481.0
129.00	254.0
129.60	253.0
130.20	752.0
131.00	218.0
140.10	201.0
140.80	1231.0
142.90	1982.0
143.80	135.0
145.00	342.0
146.00	117.0
147.90	175.0
149.90	103.0
156.80	125.0
170.20	241.0
171.10	155.0
171.80	837.0
174.00	66040.0
175.00	4751.0
176.00	66040.0
176.90	4448.0
260.70	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB197