

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050820\
 Data File : VV015956.D
 Acq On : 08 May 2020 11:39
 Operator : SY/MD
 Sample : L2520-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41W2

Quant Time: May 09 01:34:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 09 00:44:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	143114	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	141955	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	65780	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	36462	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.58	69	35960	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.80%
11) 1,1-Dichloroethene-d2	2.12	63	59703	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.60%
20) 2-Butanone-d5	3.93	46	112651	50.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.74%
24) Chloroform-d	4.38	84	87510	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
26) 1,2-Dichloroethane-d4	5.06	65	49473	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.08	84	169335	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.09	67	54122	5.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.00%
41) Toluene-d8	7.34	98	153787	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
45) trans-1,3-Dichloropropene-	7.65	79	18778	4.64	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.80%
48) 2-Hexanone-d5	8.11	63	84036	47.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.54%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	35715	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	57528	5.39	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	4020	2.752 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050820\
Data File : VV015956.D
Acq On : 08 May 2020 11:39
Operator : SY/MD
Sample : L2520-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41W2

Quant Time: May 09 01:34:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 09 00:44:25 2020
Response via : Initial Calibration

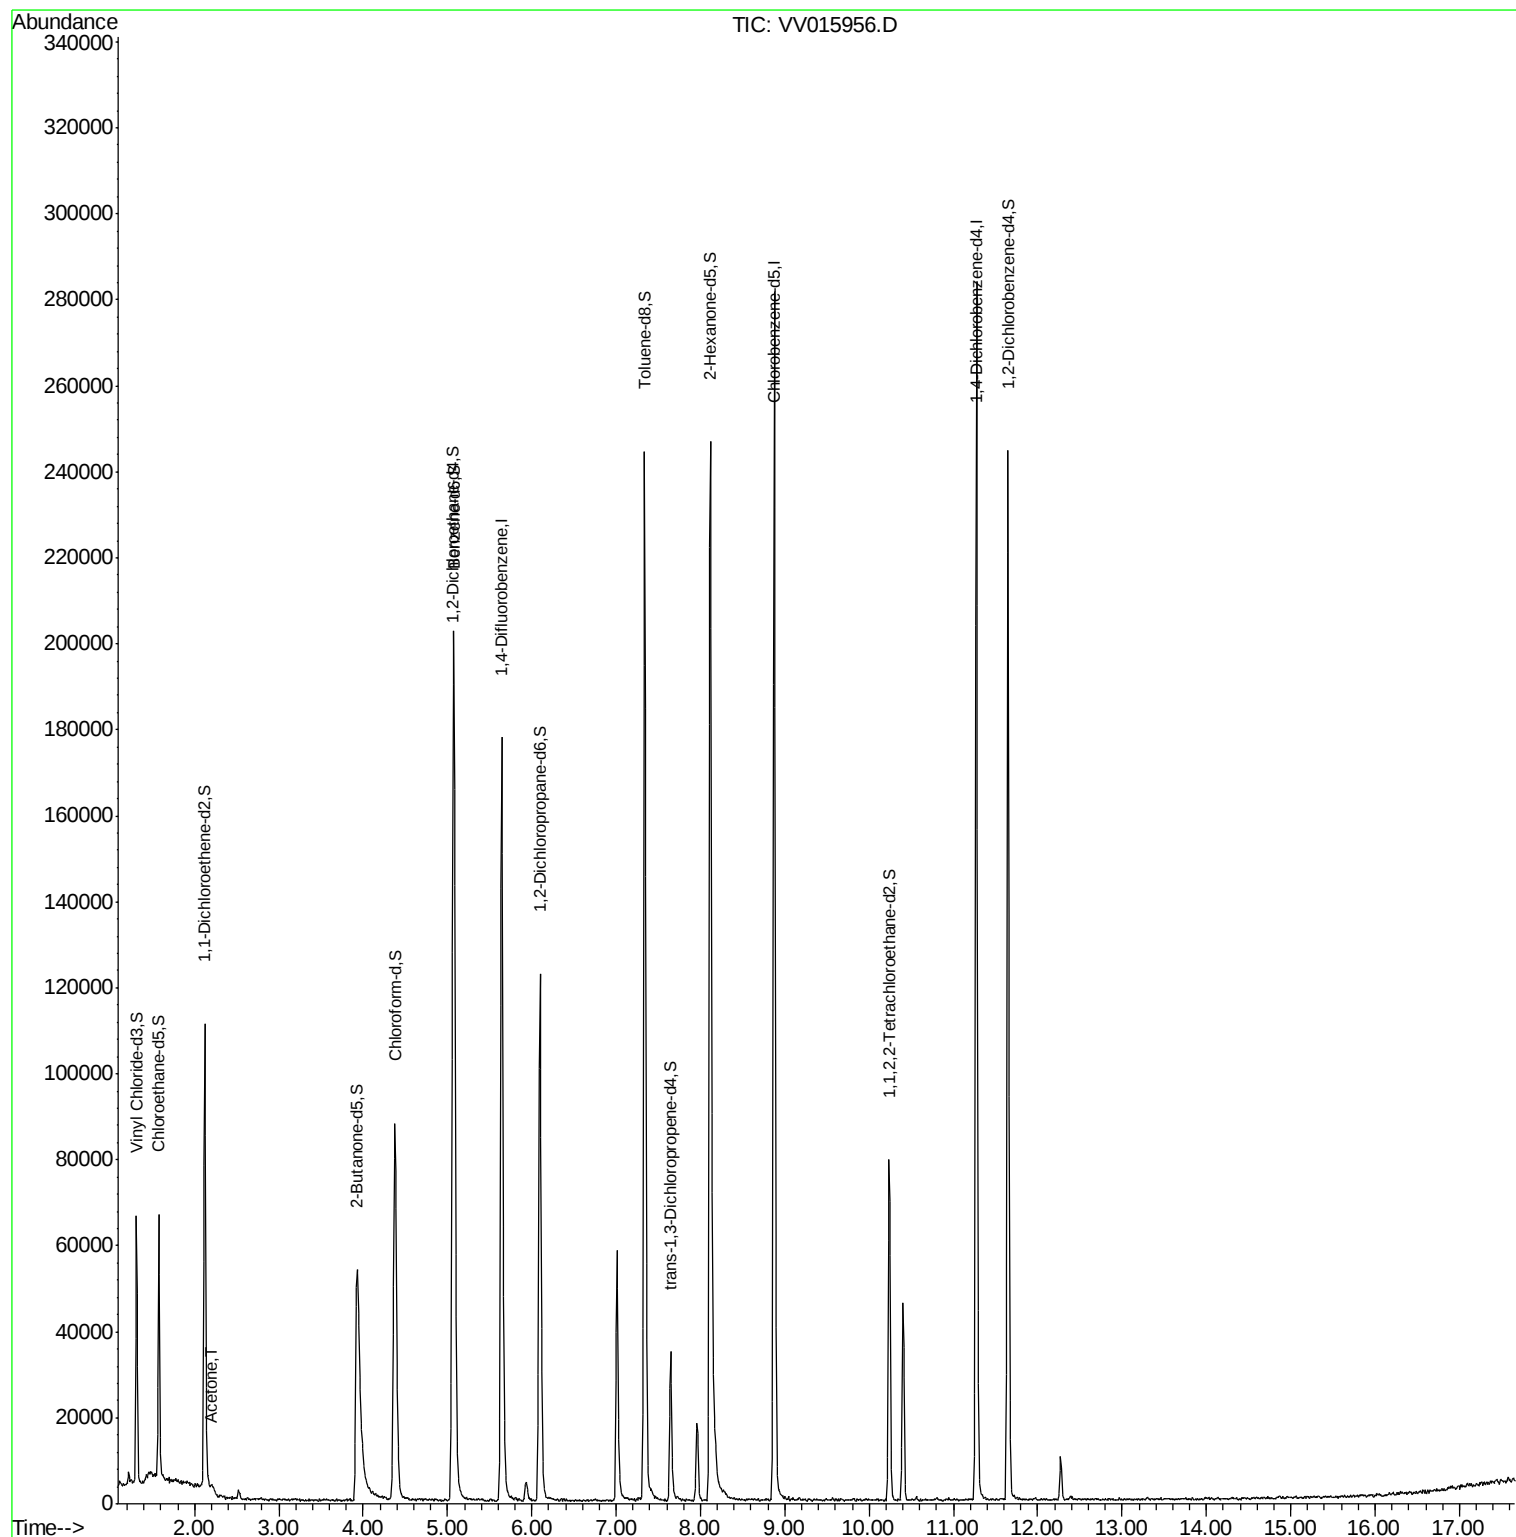

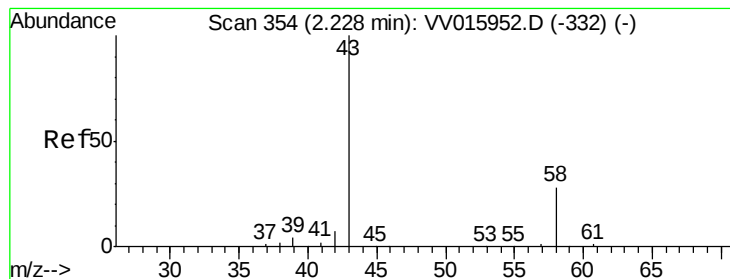

#13

Acetone

Concen: 2.752 ug/L

RT: 2.20 min Scan# 346

Delta R.T. -0.03 min

Lab File: VV015956.D

Acq: 08 May 2020 11:39

Instrument :
MSVOA_V
ClientSampleId :
H41W2

Tot Ion: 43 Resp: 4020

Ion Ratio Lower Upper

43 100

58 17.2 0.0 30.8

