

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050820\
 Data File : VV015957.D
 Acq On : 08 May 2020 12:03
 Operator : SY/MD
 Sample : L2520-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41W8

Quant Time: May 09 01:39:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 09 00:44:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	143497	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	139693	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	64652	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	34244	4.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.00%
7) Chloroethane-d5	1.58	69	33844	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.12	63	56648	3.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.60%
20) 2-Butanone-d5	3.93	46	110216	49.63	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.26%
24) Chloroform-d	4.38	84	83931	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.06	65	48631	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
32) Benzene-d6	5.08	84	162448	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.09	67	51583	5.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.60%
41) Toluene-d8	7.34	98	146523	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
45) trans-1,3-Dichloropropene-	7.65	79	18257	4.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.80%
48) 2-Hexanone-d5	8.12	63	80167	45.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.66%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	33431	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	54516	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	7106	4.851 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050820\
Data File : VV015957.D
Acq On : 08 May 2020 12:03
Operator : SY/MD
Sample : L2520-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41W8

Quant Time: May 09 01:39:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 09 00:44:25 2020
Response via : Initial Calibration

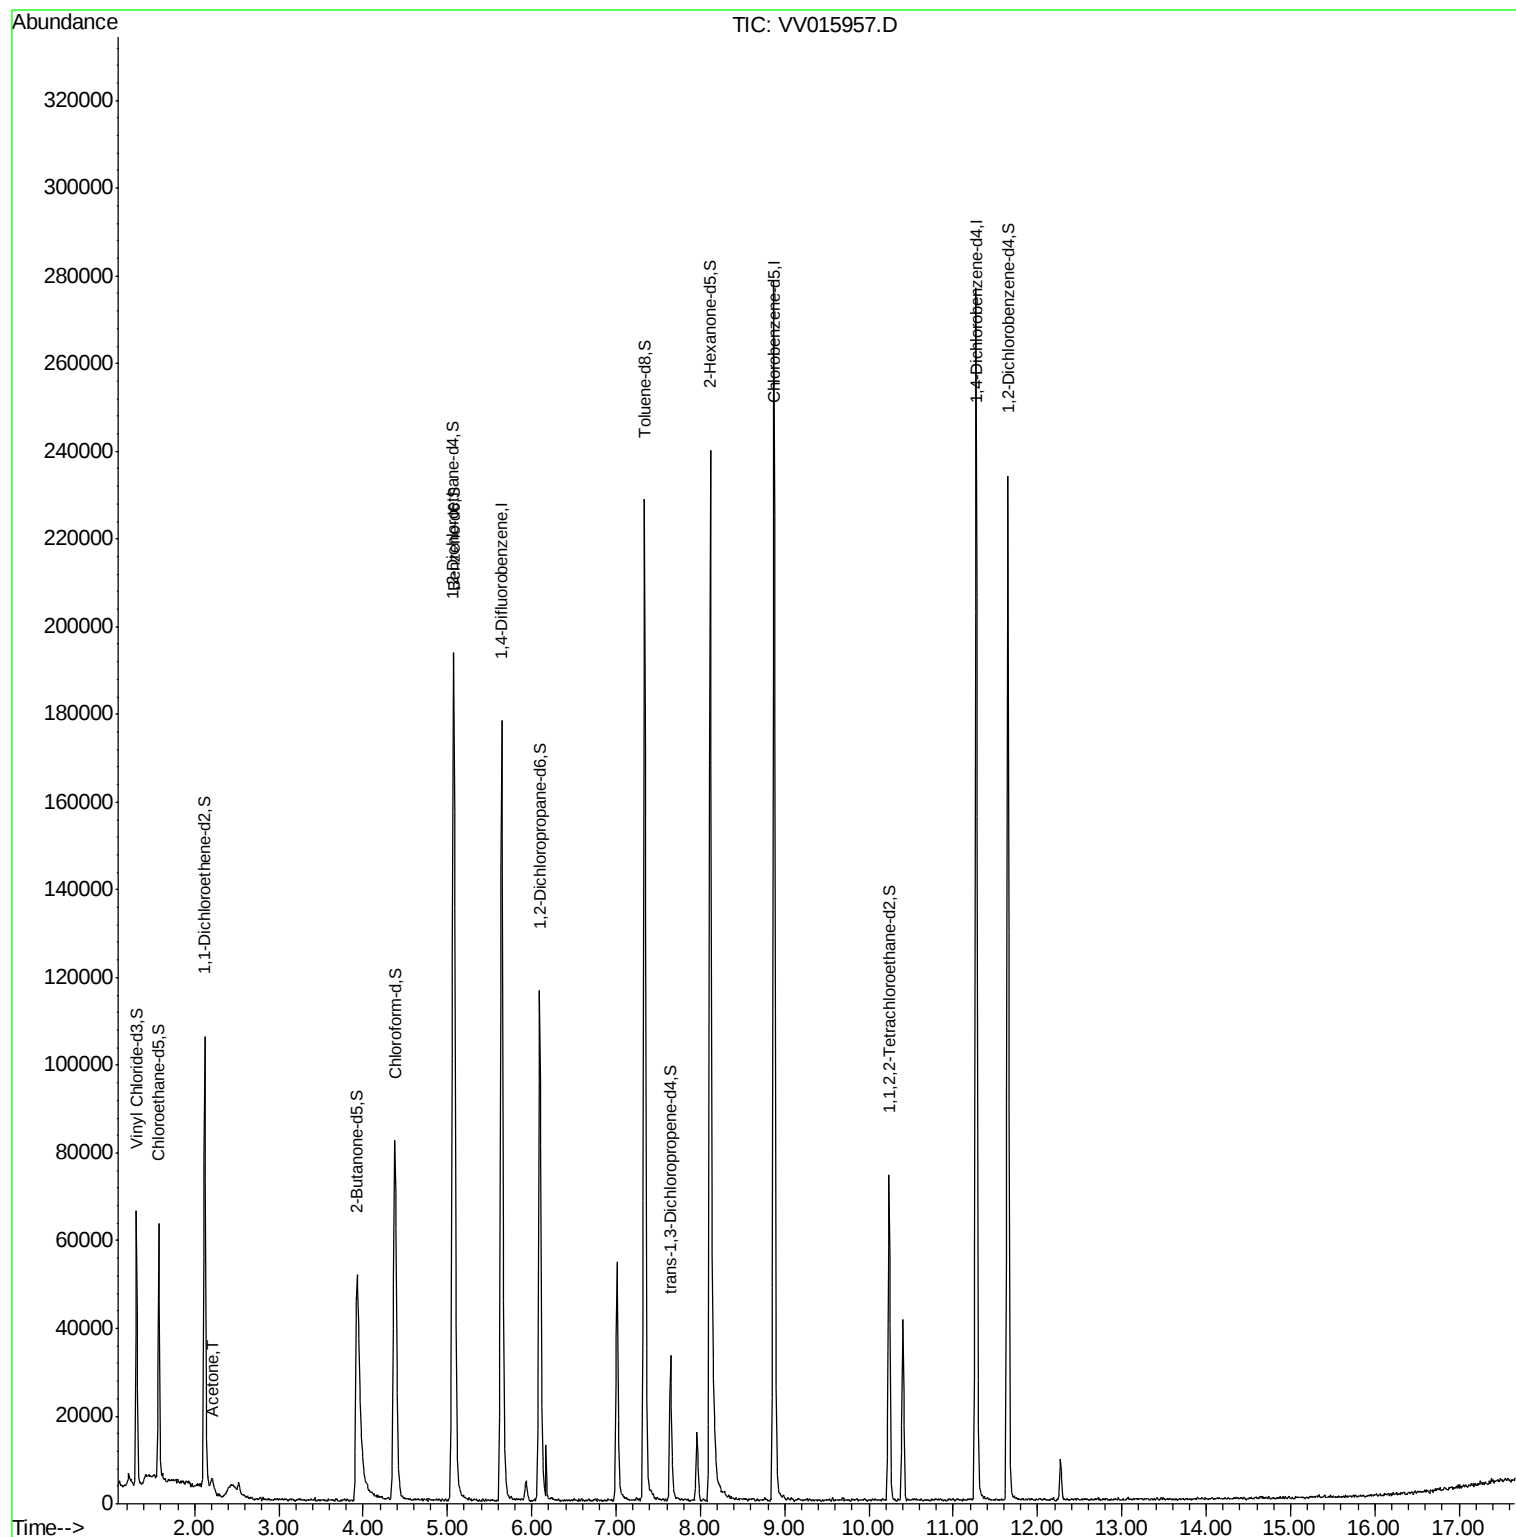

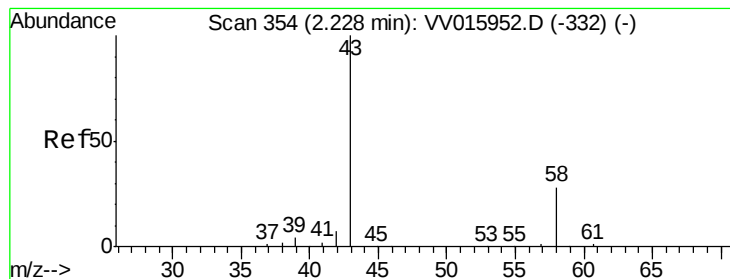

#13

Acetone

Concen: 4.851 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.02 min

Lab File: VV015957.D

Acq: 08 May 2020 12:03

Instrument :
MSVOA_V
ClientSampleId :
H41W8

Tot Ion: 43 Resp: 7106

Ion Ratio Lower Upper

43 100

58 12.1 0.0 30.8

