

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050820\
 Data File : VV015958.D
 Acq On : 08 May 2020 12:26
 Operator : SY/MD
 Sample : L2520-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41W3

Quant Time: May 09 01:45:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 09 00:44:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	141211	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	138647	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	63699	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	34095	4.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.00%
7) Chloroethane-d5	1.58	69	34795	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.80%
11) 1,1-Dichloroethene-d2	2.12	63	57134	3.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.40%
20) 2-Butanone-d5	3.92	46	108930	49.85	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.70%
24) Chloroform-d	4.38	84	84333	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
26) 1,2-Dichloroethane-d4	5.06	65	47780	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.08	84	158889	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
36) 1,2-Dichloropropane-d6	6.09	67	50215	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.34	98	144004	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
45) trans-1,3-Dichloropropene-	7.64	79	18390	4.65	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.00%
48) 2-Hexanone-d5	8.11	63	79266	45.65	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.30%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	32834	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	53781	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	4380	3.038 ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050820\
Data File : VV015958.D
Acq On : 08 May 2020 12:26
Operator : SY/MD
Sample : L2520-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41W3

Quant Time: May 09 01:45:28 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 09 00:44:25 2020
Response via : Initial Calibration

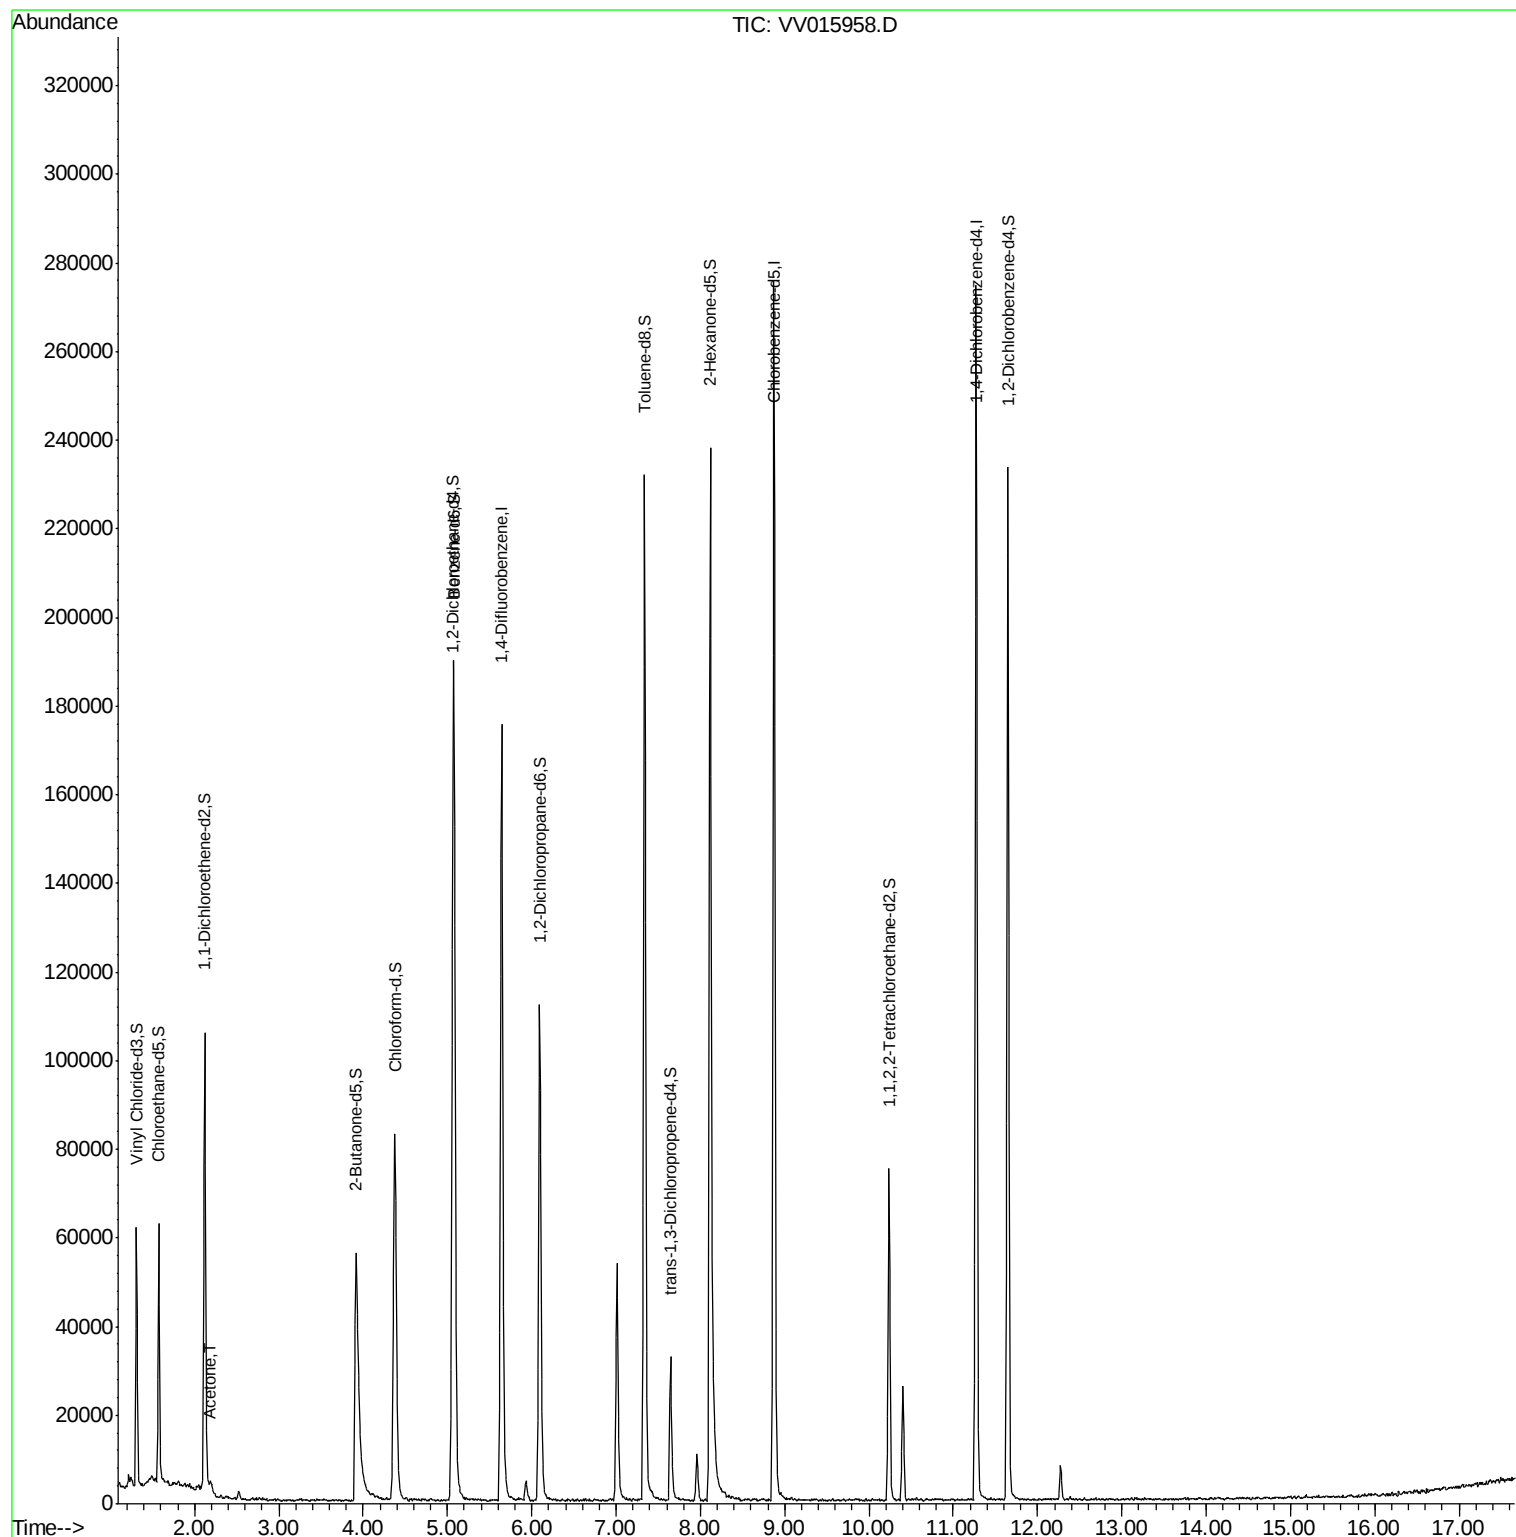

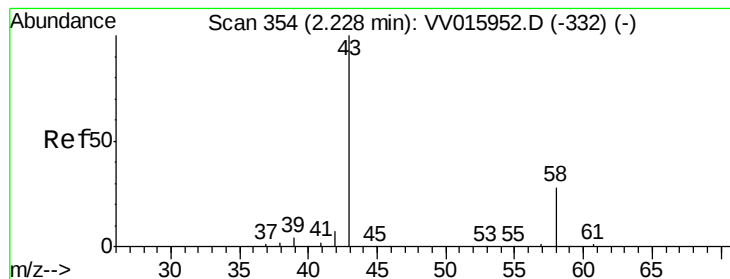

#13

Acetone

Concen: 3.038 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.04 min

Lab File: VV015958.D

Acq: 08 May 2020 12:26

Instrument :
MSVOA_V
ClientSampleId :
H41W3

Tot Ion: 43 Resp: 4380

Ion Ratio Lower Upper

43 100

58 31.9 0.0 30.8#

