

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050820\
 Data File : VV015960.D
 Acq On : 08 May 2020 13:12
 Operator : SY/MD
 Sample : L2520-18
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41W5

Quant Time: May 09 02:01:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 09 00:44:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	149545	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	145371	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	68273	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34920	4.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.00%
7) Chloroethane-d5	1.58	69	35282	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.12	63	57522	3.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.00%
20) 2-Butanone-d5	3.92	46	112807	48.75	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.50%
24) Chloroform-d	4.38	84	86230	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	5.06	65	48806	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
32) Benzene-d6	5.08	84	164040	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	6.10	67	52239	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	7.34	98	148896	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
45) trans-1,3-Dichloropropene-	7.65	79	18049	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
48) 2-Hexanone-d5	8.11	63	82660	45.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.82%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	35080	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	56536	5.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	6881	4.507 ug/L	# 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050820\
Data File : VV015960.D
Acq On : 08 May 2020 13:12
Operator : SY/MD
Sample : L2520-18
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41W5

Quant Time: May 09 02:01:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 09 00:44:25 2020
Response via : Initial Calibration

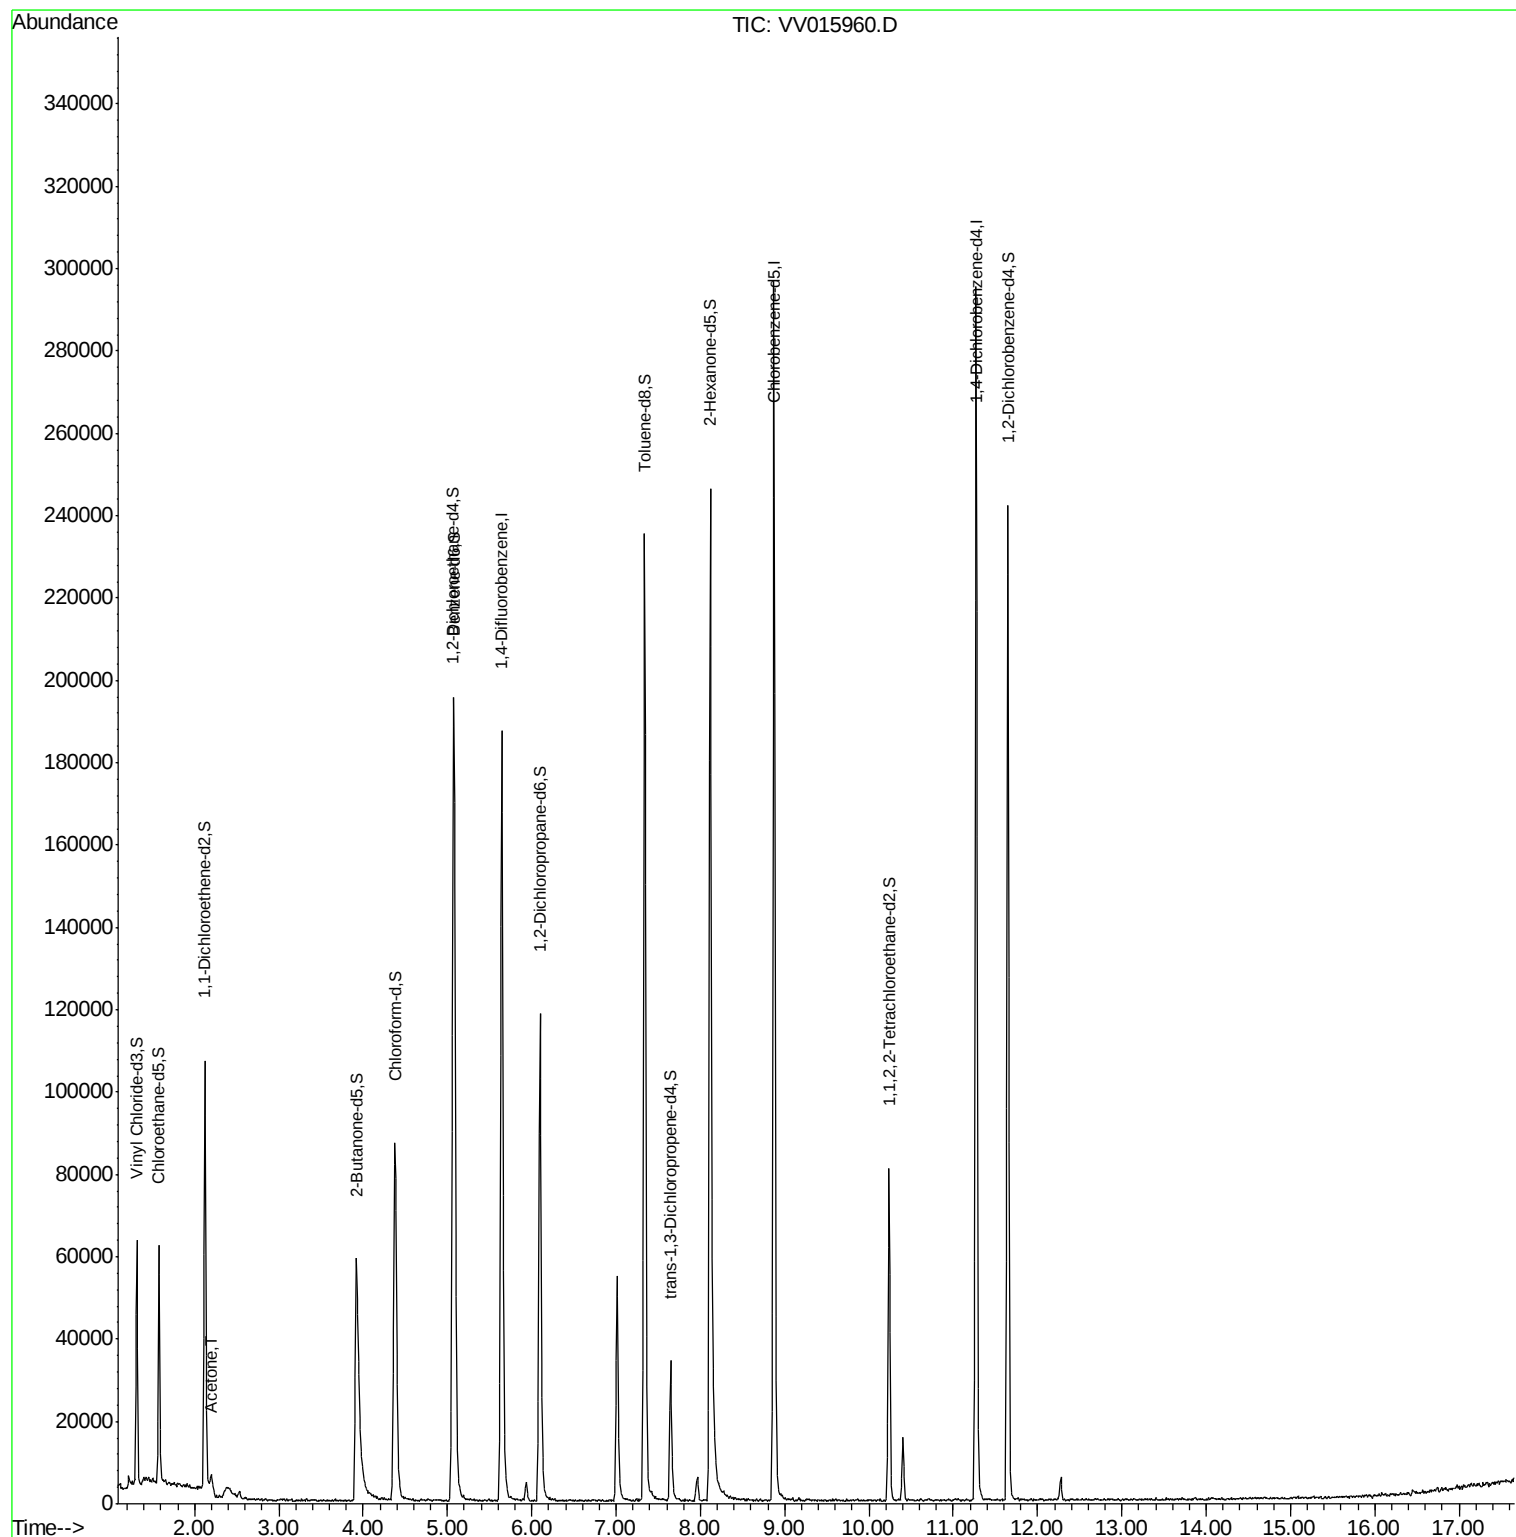

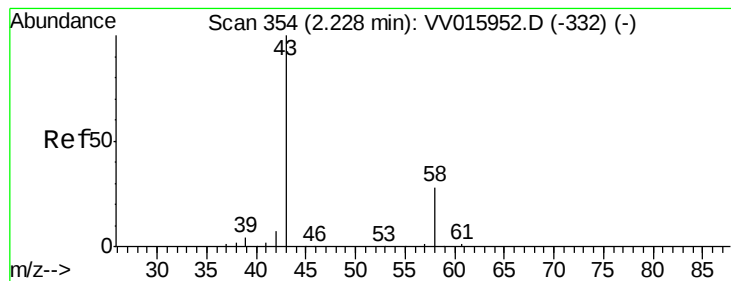

#13
 Acetone
 Concen: 4.507 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. -0.03 min
 Lab File: VV015960.D
 Acq: 08 May 2020 13:12

Instrument :
 MSVOA_V
 ClientSampleId :
 H41W5

Tot Ion: 43 Resp: 6881
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 30.8#

