

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050820\
 Data File : VV015962.D
 Acq On : 08 May 2020 13:59
 Operator : SY/MD
 Sample : L2541-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41X0

Quant Time: May 09 02:10:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 09 00:44:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	145636	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	144519	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	67058	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34645	4.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.60%
7) Chloroethane-d5	1.58	69	34476	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.00%
11) 1,1-Dichloroethene-d2	2.12	63	57095	3.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.20%
20) 2-Butanone-d5	3.91	46	108220	48.02	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.04%
24) Chloroform-d	4.38	84	82877	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.06	65	48641	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.08	84	162017	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.10	67	51689	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.34	98	145049	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.20%
45) trans-1,3-Dichloropropene-	7.65	79	17351	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
48) 2-Hexanone-d5	8.11	63	82757	45.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.46%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	34733	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	55988	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds				Ovalue
13) Acetone	2.20	43	4119	2.771 ug/L # 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050820\
Data File : VV015962.D
Acq On : 08 May 2020 13:59
Operator : SY/MD
Sample : L2541-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41X0

Quant Time: May 09 02:10:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 09 00:44:25 2020
Response via : Initial Calibration

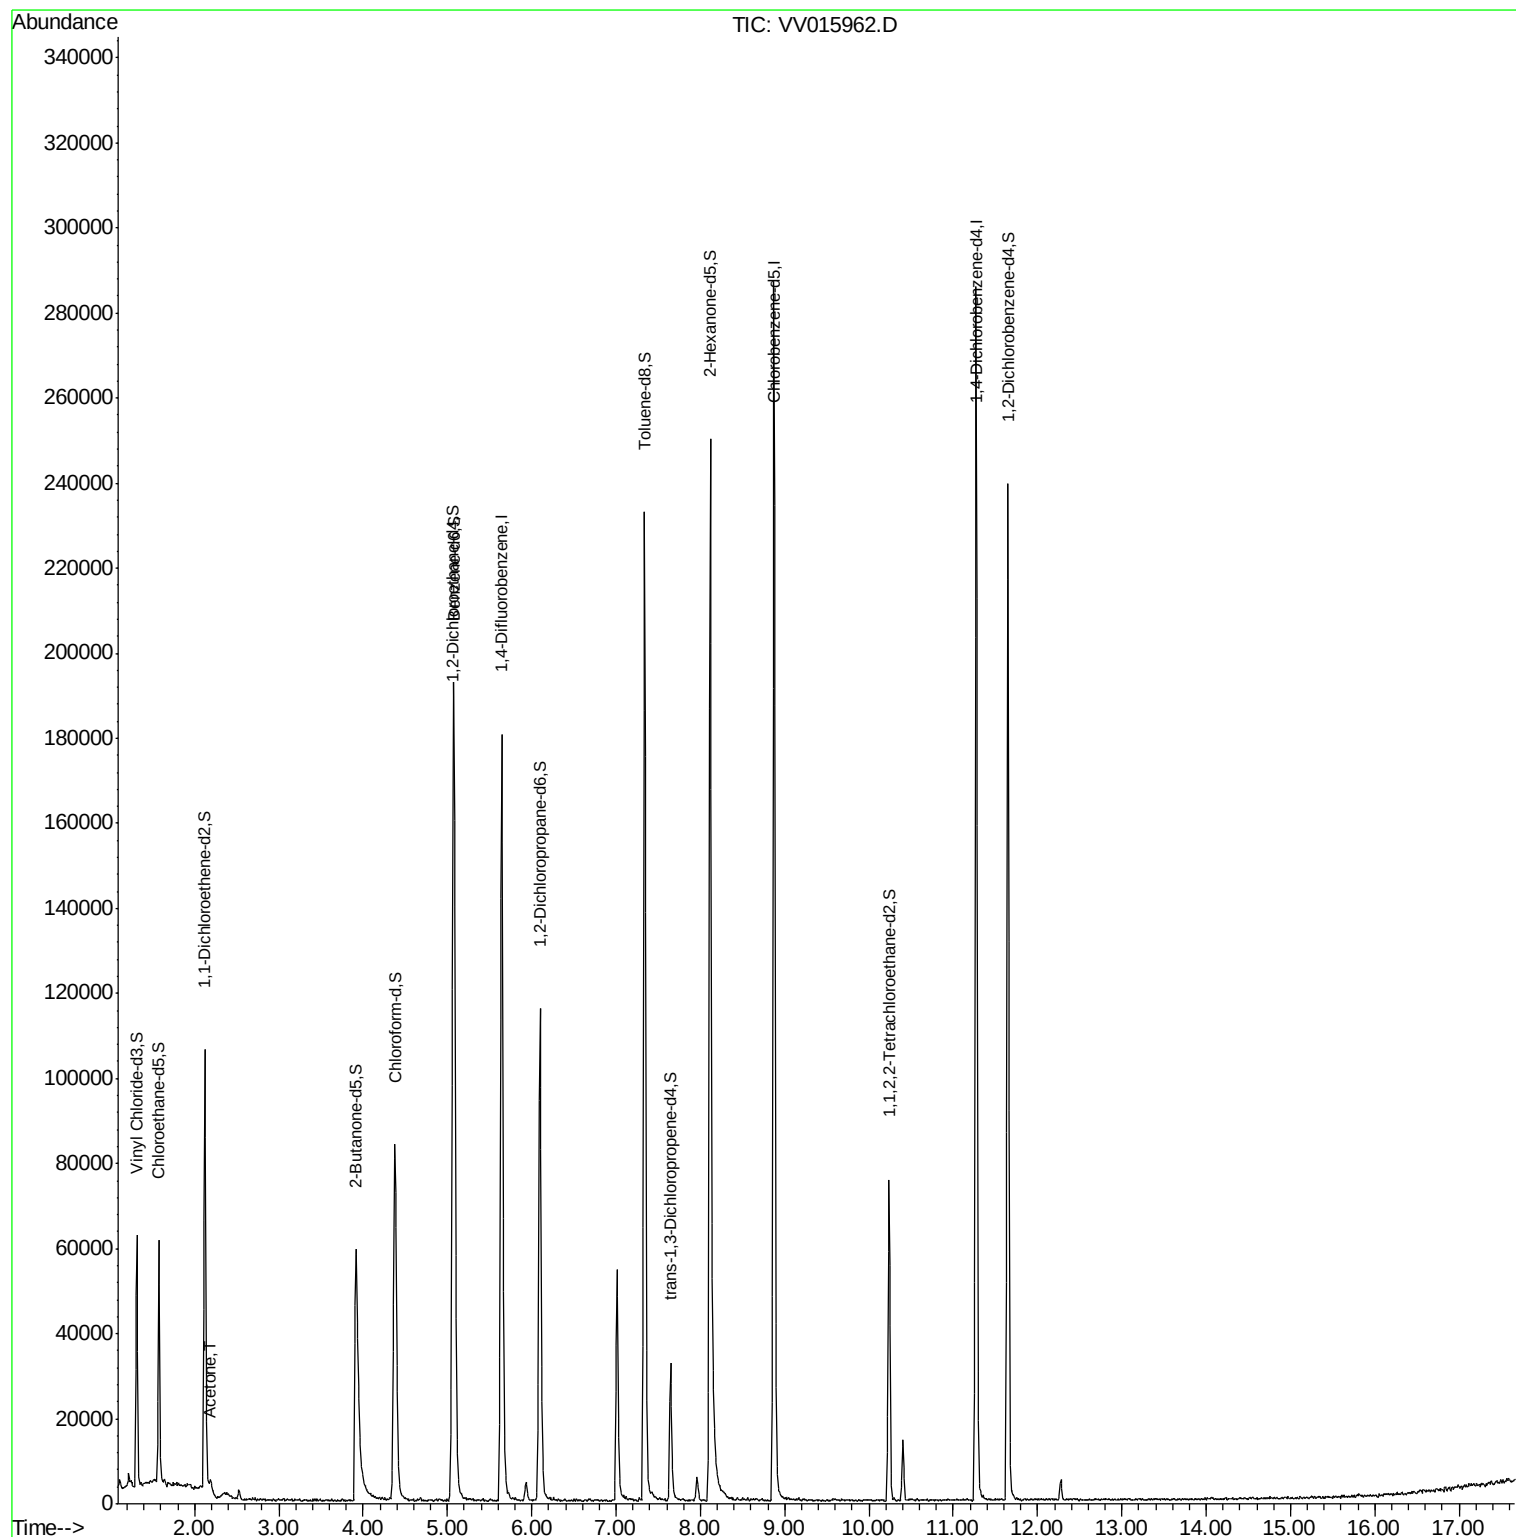

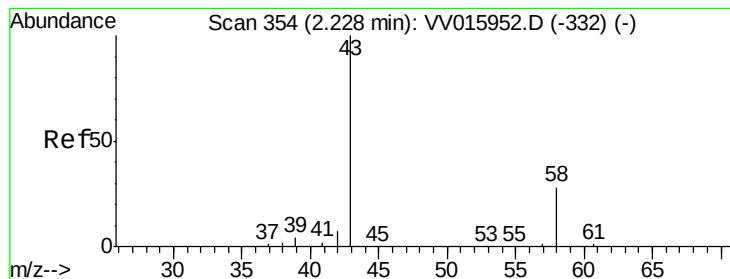

#13

Acetone

Concen: 2.771 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.03 min

Lab File: VV015962.D

Acq: 08 May 2020 13:59

Instrument :
MSVOA_V
ClientSampleId :
H41X0

Tot Ion: 43 Resp: 4119

Ion Ratio Lower Upper

43 100

58 33.2 0.0 30.8#

