

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050820\
 Data File : VV015964.D
 Acq On : 08 May 2020 14:46
 Operator : SY/MD
 Sample : L2520-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41X8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.113	3	7	10	rBV2	6136	5327	1.00%	0.109%
2	1.142	10	16	34	rVB	480054	452963	85.31%	9.270%
3	1.315	61	70	80	rVB	61170	65469	12.33%	1.340%
4	1.579	144	152	162	rBV	58959	67936	12.80%	1.390%
5	2.122	311	321	335	rVB	106645	157919	29.74%	3.232%
6	3.929	870	883	917	rBV2	56734	198164	37.32%	4.056%
7	4.376	1006	1022	1050	rBV	83509	219716	41.38%	4.497%
8	5.074	1222	1239	1268	rBV2	196678	495695	93.36%	10.145%
9	5.643	1404	1416	1443	rBV	181502	373102	70.27%	7.636%
10	5.942	1499	1509	1527	rVB7	8944	19895	3.75%	0.407%
11	6.093	1543	1556	1578	rBV	117814	244564	46.06%	5.005%
12	7.010	1830	1841	1861	rBV2	56100	104738	19.73%	2.144%
13	7.338	1932	1943	1964	rBV	236386	415021	78.17%	8.494%
14	7.646	2029	2039	2058	rBV	33928	62151	11.71%	1.272%
15	8.000	2143	2149	2161	rVB4	6748	11498	2.17%	0.235%
16	8.116	2173	2185	2219	rBV	255108	530950	100.00%	10.866%
17	8.874	2407	2421	2439	rBV	290733	473288	89.14%	9.686%
18	10.238	2835	2845	2860	rBV2	81667	130632	24.60%	2.673%
19	10.402	2888	2896	2912	rVB4	6512	10002	1.88%	0.205%
20	11.270	3156	3166	3185	rBV	293520	450964	84.94%	9.229%
21	11.646	3272	3283	3298	rBV	245322	385491	72.60%	7.889%
22	12.373	3502	3509	3518	rBV5	7329	10794	2.03%	0.221%


Sum of corrected areas: 4886279

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050820\
Data File : VV015964.D
Acq On : 08 May 2020 14:46
Operator : SY/MD
Sample : L2520-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41X8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

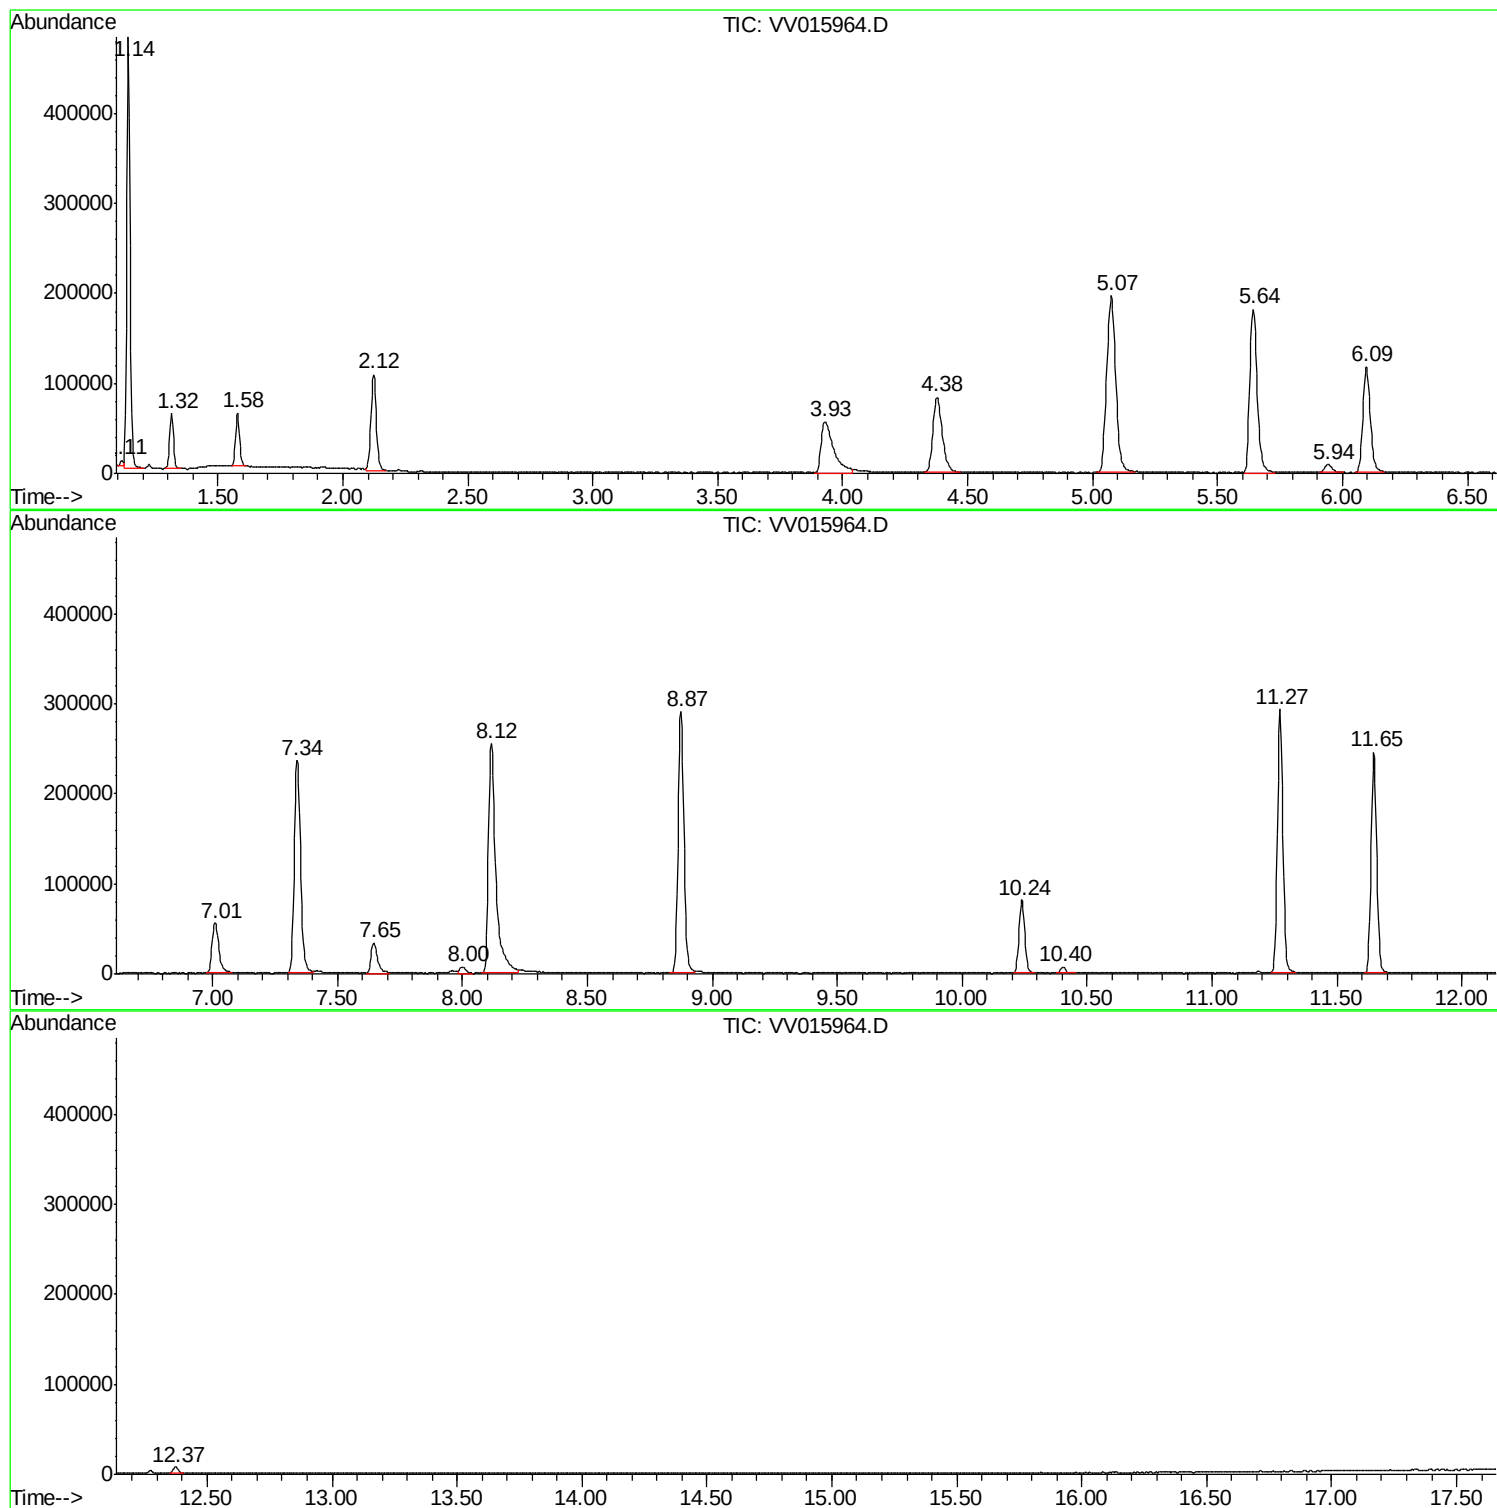

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV050820\
Data File : VV015964.D
Acq On : 08 May 2020 14:46
Operator : SY/MD
Sample : L2520-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41X8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV050820\
Data File : VV015964.D
Acq On : 08 May 2020 14:46
Operator : SY/MD
Sample : L2520-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41X8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc