




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
 Data File : VV031007.D
 Acq On : 08 May 2023 14:14
 Operator : SY/MD
 Sample : 02613-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 09 01:34:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 06 01:44:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/09/2023
 Supervised By :Mahesh Dadoda 05/09/2023

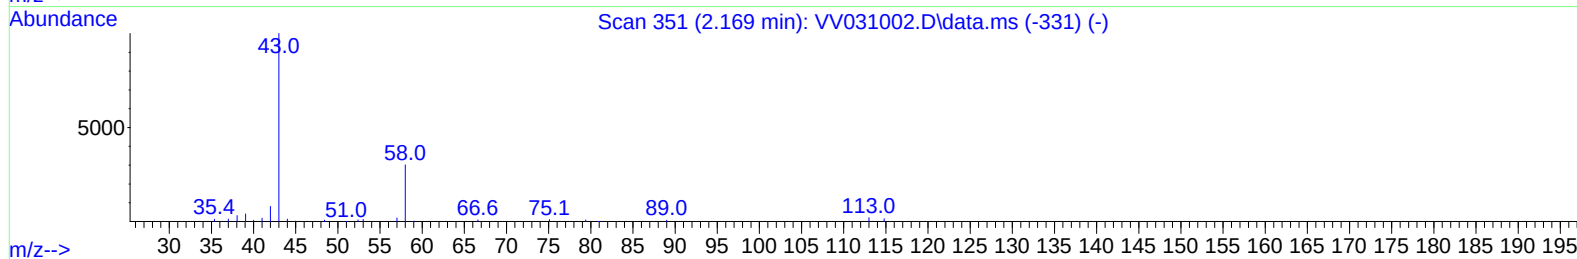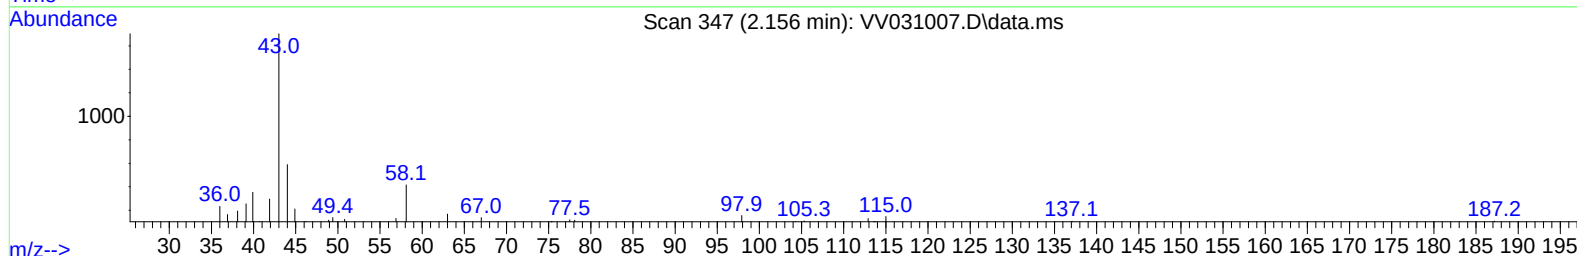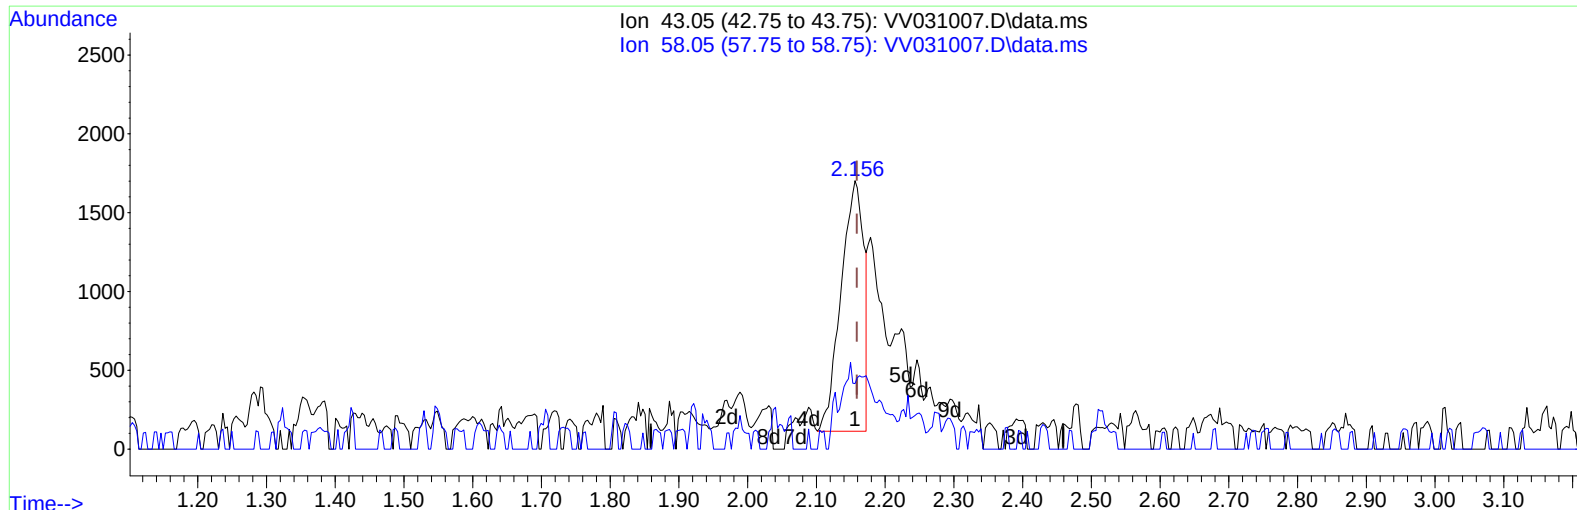

TIC: VV031007.D\data.ms

(13) Acetone (T)

2.156min (-0.003) 2.23 ug/L

response 3643

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	18.50	32.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
 Data File : VV031007.D
 Acq On : 08 May 2023 14:14
 Operator : SY/MD
 Sample : 02613-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 09 01:34:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 06 01:44:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/09/2023
 Supervised By :Mahesh Dadoda 05/09/2023

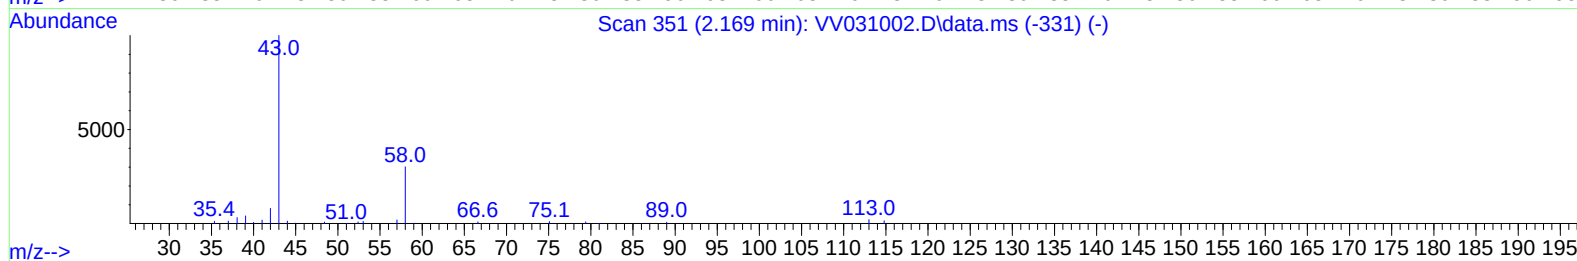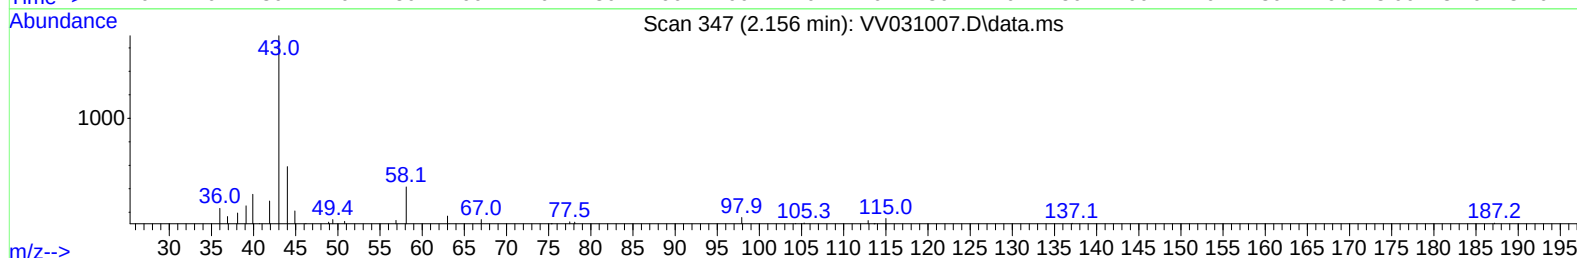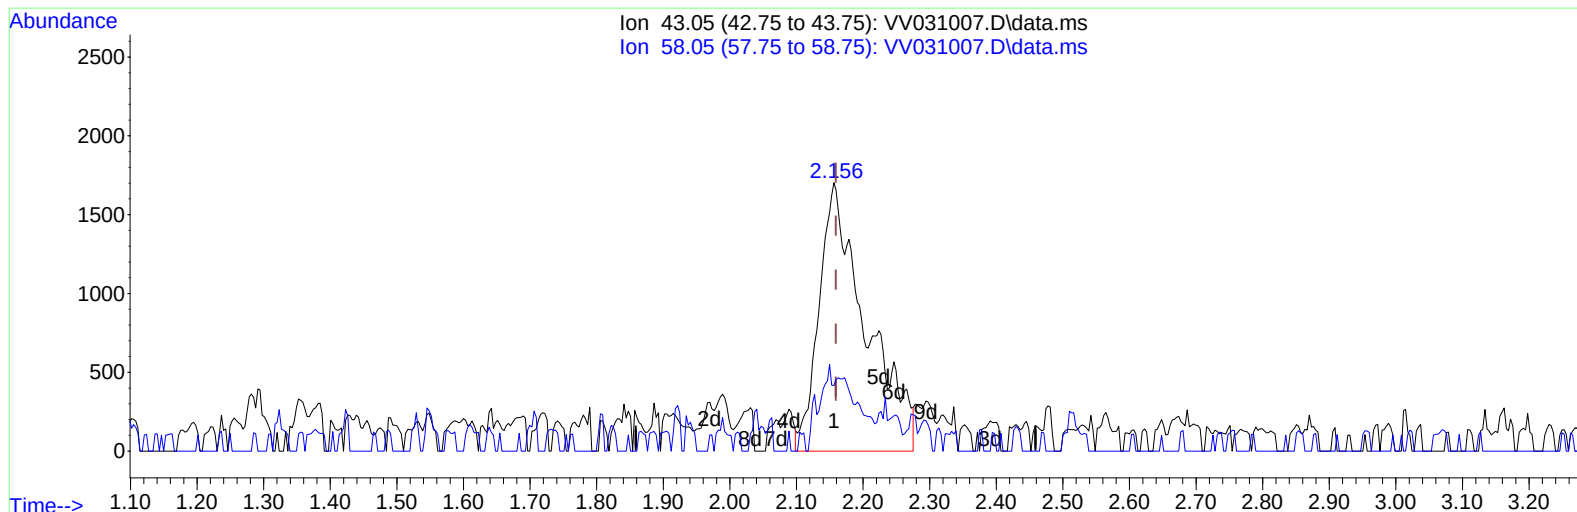

TIC: VV031007.D\data.ms

(13) Acetone (T)

2.156min (-0.003) 5.06 ug/L m

response	8265	
Ion	Exp%	Act%
43.05	100.00	100.00
58.05	18.50	14.42
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
 Data File : VV031007.D
 Acq On : 08 May 2023 14:14
 Operator : SY/MD
 Sample : 02613-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/09/2023
 Supervised By :Mahesh Dadoda 05/09/2023

Quant Time: May 09 01:34:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 06 01:44:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	130788	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	127480	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	62480	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	50092	4.649	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.000%	
7) Chloroethane-d5	1.539	69	46555	5.296	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	106.000%	
11) 1,1-Dichloroethene-d2	2.063	65	27471	4.817	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	96.400%	
20) 2-Butanone-d5	3.831	46	101547	53.143	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.280%	
24) Chloroform-d	4.259	84	108475	5.065	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	4.953	65	58266	5.352	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.000%	
32) Benzene-d6	4.970	84	190054	5.086	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.800%	
36) 1,2-Dichloropropane-d6	5.998	67	54971	5.059	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.200%	
41) Toluene-d8	7.249	98	161584	4.541	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
43) trans-1,3-Dichloroprop...	7.561	79	19090	4.687	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.800%	
46) 2-Hexanone-d5	8.037	63	70567	49.451	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.900%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	42111	5.347	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	107.000%	
66) 1,2-Dichlorobenzene-d4	11.571	152	61119	5.248	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	105.000%	
Target Compounds					Qvalue	
13) Acetone	2.156	43	8265m	5.064	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031007.D
Acq On : 08 May 2023 14:14
Operator : SY/MD
Sample : 02613-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 09 01:34:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 06 01:44:36 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/09/2023
Supervised By :Mahesh Dadoda 05/09/2023

