

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
 Data File : VV031004.D
 Acq On : 08 May 2023 12:54
 Operator : SY/MD
 Sample : 02613-04DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	88	rBV	59173	70048	15.84%	1.737%
2	1.535	144	154	164	rBV	59670	71638	16.20%	1.776%
3	2.063	308	318	331	rBV2	167677	282093	63.80%	6.993%
4	2.452	429	439	451	rBV3	16661	32355	7.32%	0.802%
5	3.124	633	648	660	rBV2	18749	42681	9.65%	1.058%
6	3.841	855	871	890	rBV2	25068	107375	24.28%	2.662%
7	4.259	985	1001	1019	rBV	91374	226956	51.33%	5.626%
8	4.519	1066	1082	1101	rBV2	89553	231510	52.36%	5.739%
9	4.966	1203	1221	1243	rBV2	168242	442161	100.00%	10.961%
10	5.542	1388	1400	1417	rBV2	132275	283430	64.10%	7.026%
11	5.841	1481	1493	1514	rBV3	54609	116837	26.42%	2.896%
12	5.998	1530	1542	1558	rBV2	103240	220511	49.87%	5.467%
13	6.921	1816	1829	1850	rBV	42551	94037	21.27%	2.331%
14	7.249	1917	1931	1947	rBV	175225	316084	71.49%	7.836%
15	7.561	2020	2028	2044	rBV2	25637	52819	11.95%	1.309%
16	8.037	2166	2176	2216	rBV	142371	377412	85.36%	9.356%
17	8.792	2398	2411	2431	rBV	197499	343412	77.67%	8.513%
18	10.162	2826	2837	2854	rBV2	77371	128538	29.07%	3.187%
19	10.336	2881	2891	2900	rBV4	5827	11343	2.57%	0.281%
20	10.860	3046	3054	3059	rBV10	4943	7369	1.67%	0.183%
21	11.194	3147	3158	3176	rBV	161477	274924	62.18%	6.815%
22	11.567	3261	3274	3291	rBV	148489	249088	56.33%	6.175%
23	12.596	3584	3594	3605	rVB7	9168	17014	3.85%	0.422%
24	13.210	3776	3785	3794	rBV9	11500	20562	4.65%	0.510%
25	13.692	3928	3935	3947	rVB9	8862	13624	3.08%	0.338%




Sum of corrected areas: 4033821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031004.D
Acq On : 08 May 2023 12:54
Operator : SY/MD
Sample : 02613-04DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

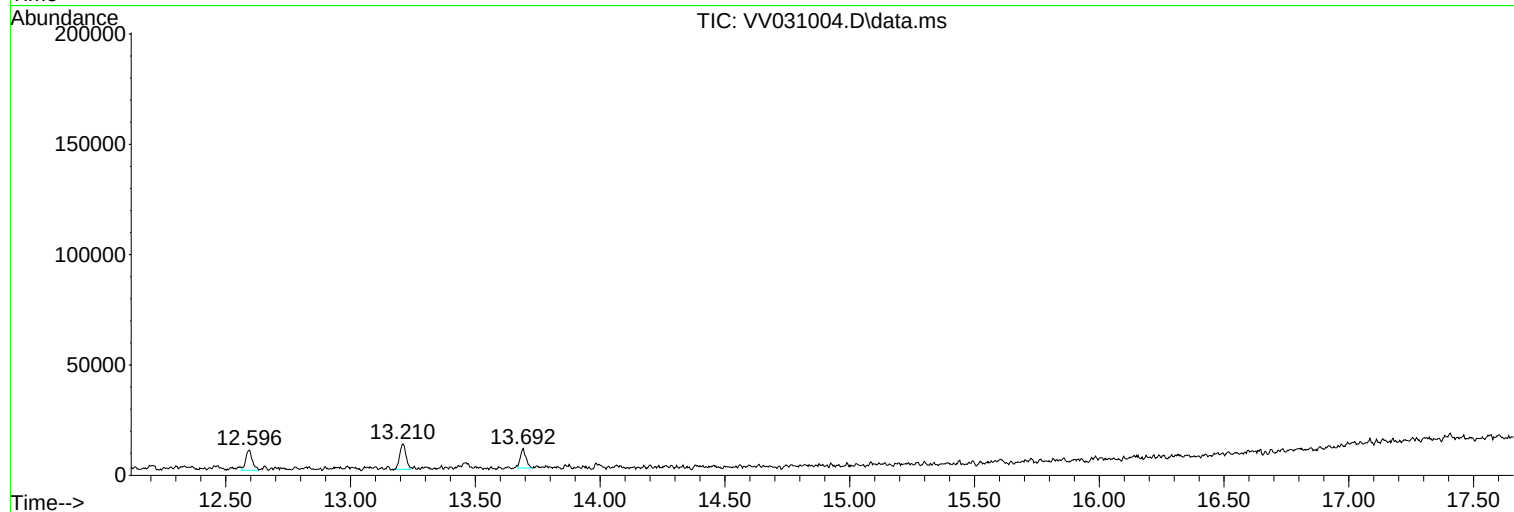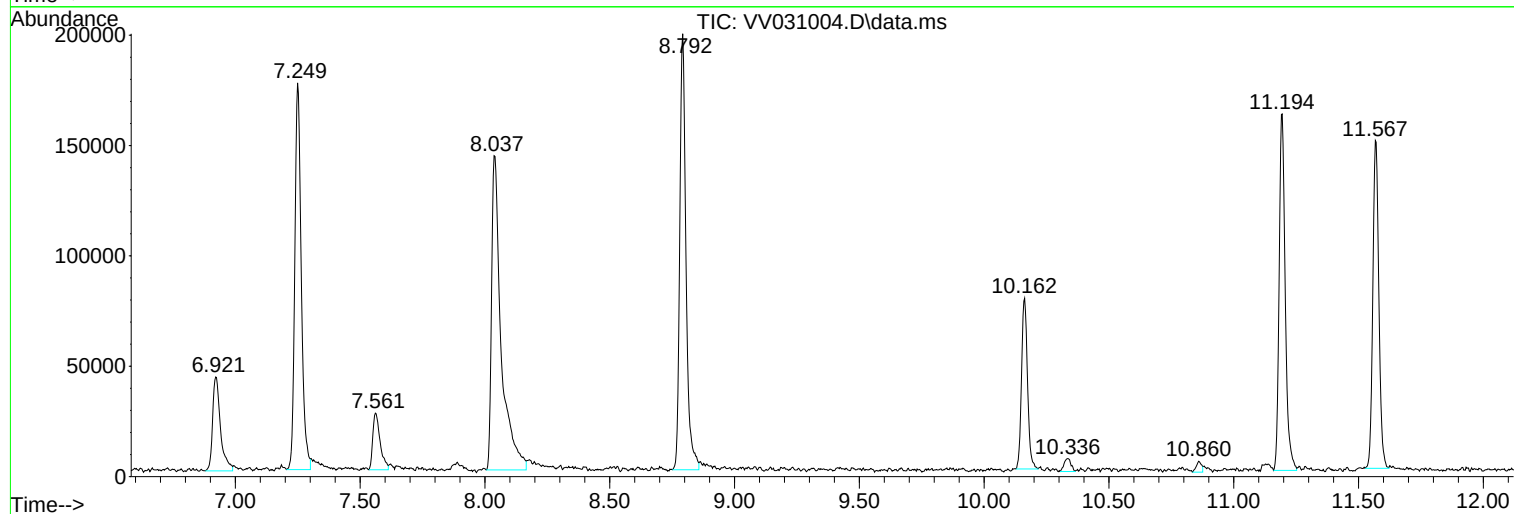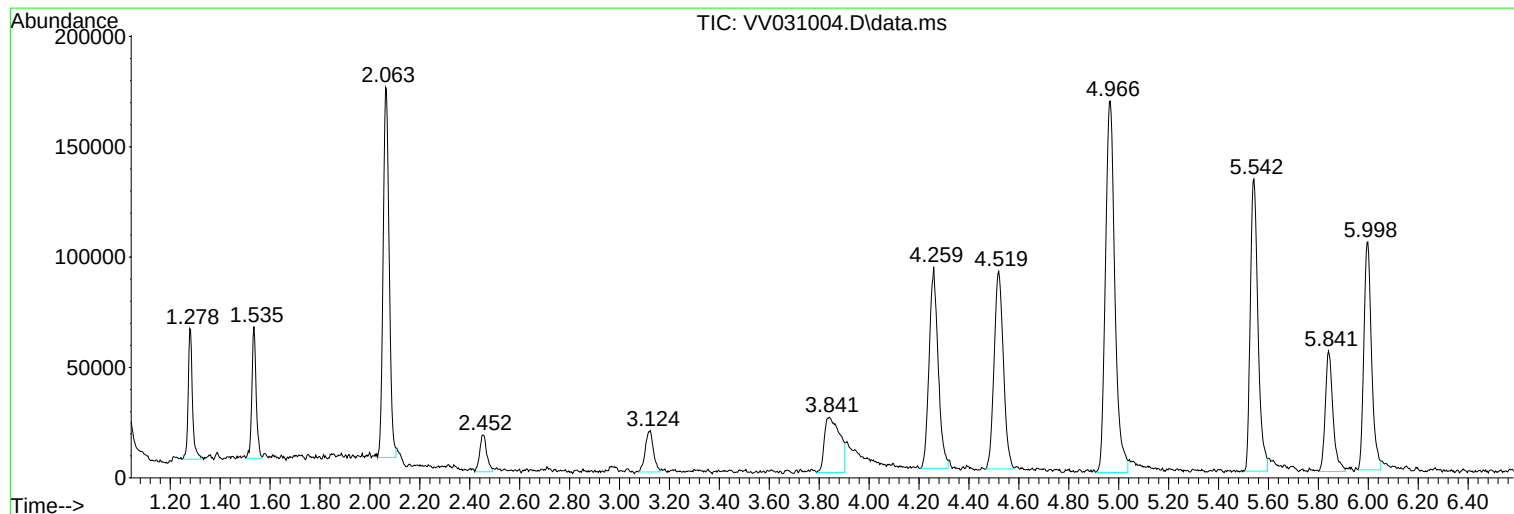

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031004.D
Acq On : 08 May 2023 12:54
Operator : SY/MD
Sample : 02613-04DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031004.D
Acq On : 08 May 2023 12:54
Operator : SY/MD
Sample : 02613-04DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc