

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
 Data File : VV031005.D
 Acq On : 08 May 2023 13:16
 Operator : SY/MD
 Sample : 02614-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 X3G07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	15	21	33	rVB	74092	73799	8.55%	0.710%
2	1.285	69	76	92	rBV2	134496	158291	18.33%	1.524%
3	1.555	146	160	174	rBV2	165574	278324	32.23%	2.679%
4	2.072	307	321	333	rBV2	490205	863534	100.00%	8.312%
5	2.143	333	343	369	rVB2	91994	253864	29.40%	2.443%
6	2.391	412	420	433	rBV2	19403	38321	4.44%	0.369%
7	2.703	504	517	531	rBV	62950	112506	13.03%	1.083%
8	3.121	633	647	666	rBV	36558	80521	9.32%	0.775%
9	3.825	851	866	890	rBV3	106001	309990	35.90%	2.984%
10	4.162	956	971	987	rBV3	56699	149652	17.33%	1.440%
11	4.278	989	1007	1039	rVB4	182838	630578	73.02%	6.069%
12	4.523	1066	1083	1103	rVB2	43320	115983	13.43%	1.116%
13	4.748	1135	1153	1169	rBV2	61834	156838	18.16%	1.510%
14	4.969	1205	1222	1240	rBV2	205868	530337	61.41%	5.105%
15	5.056	1242	1249	1265	rVB2	21782	49151	5.69%	0.473%
16	5.545	1386	1401	1423	rBV2	153669	335955	38.90%	3.234%
17	5.844	1481	1494	1511	rBV2	62858	134028	15.52%	1.290%
18	5.998	1529	1542	1565	rBV	123199	256419	29.69%	2.468%
19	6.921	1817	1829	1835	rBV	57207	97163	11.25%	0.935%
20	6.963	1835	1842	1863	rVB2	91762	178683	20.69%	1.720%
21	7.169	1895	1906	1921	rBV	395095	724015	83.84%	6.969%
22	7.249	1921	1931	1951	rVB	283106	508578	58.89%	4.895%
23	7.561	2017	2028	2033	rBV	38872	63725	7.38%	0.613%
24	7.590	2033	2037	2056	rVB	43905	79152	9.17%	0.762%
25	7.780	2085	2096	2112	rBV3	40714	77564	8.98%	0.747%
26	7.911	2120	2137	2150	rBV	121069	217203	25.15%	2.091%
27	8.037	2166	2176	2208	rBV	186948	401671	46.51%	3.866%
28	8.291	2245	2255	2268	rBV2	43787	77190	8.94%	0.743%
29	8.792	2400	2411	2415	rBV	252051	389302	45.08%	3.747%
30	8.821	2416	2420	2447	rVB	286367	439102	50.85%	4.226%
31	9.673	2675	2685	2702	rBV3	31244	56612	6.56%	0.545%
32	10.162	2826	2837	2858	rBV2	85503	176554	20.45%	1.699%
33	10.333	2880	2890	2902	rVB2	13338	22837	2.64%	0.220%
34	10.860	3041	3054	3067	rBV	252732	390831	45.26%	3.762%
35	11.124	3126	3136	3148	rBV	141345	229035	26.52%	2.205%
36	11.194	3148	3158	3181	rVB2	267036	565772	65.52%	5.446%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031005.D
Acq On : 08 May 2023 13:16
Operator : SY/MD
Sample : 02614-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
X3G07

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Title : TRACE VOA SFAM1.0

37	11.503	3244	3254	3264	rBV8	7234	16245	1.88%	0.156%
38	11.570	3264	3275	3294	rVB	230762	376429	43.59%	3.623%
39	12.590	3577	3592	3608	rBV	238000	372053	43.08%	3.581%
40	13.207	3773	3784	3801	rBV	160907	262519	30.40%	2.527%
41	13.689	3923	3934	3949	rBV2	86588	139104	16.11%	1.339%




Sum of corrected areas: 10389430

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031005.D
Acq On : 08 May 2023 13:16
Operator : SY/MD
Sample : 02614-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
X3G07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

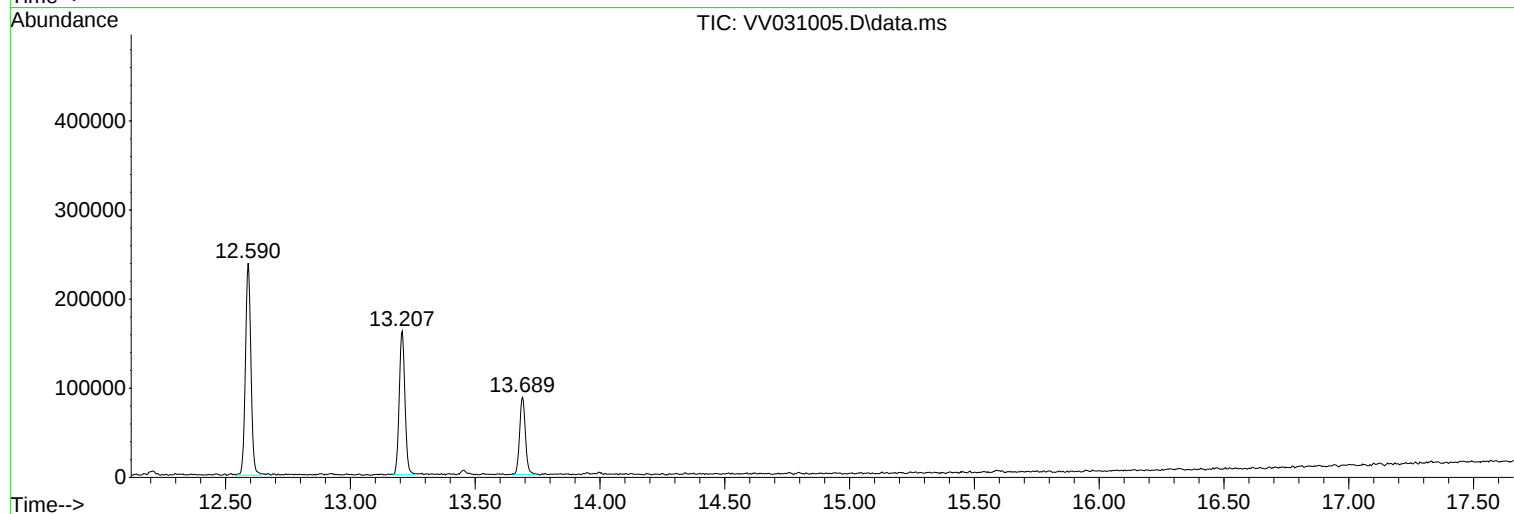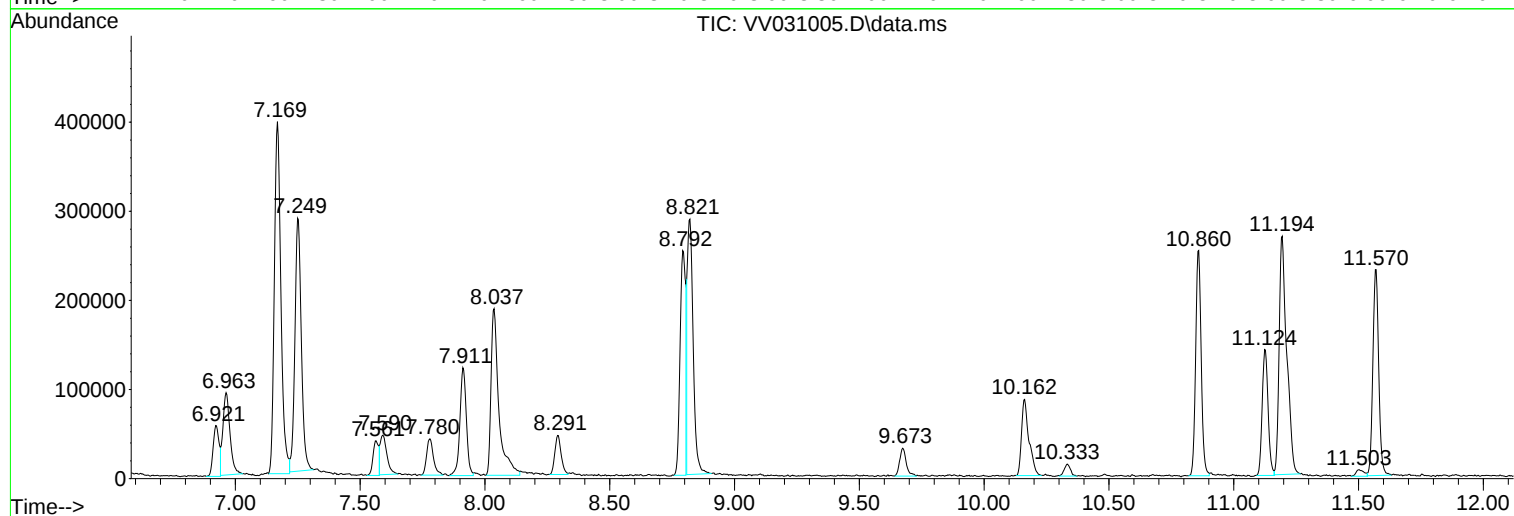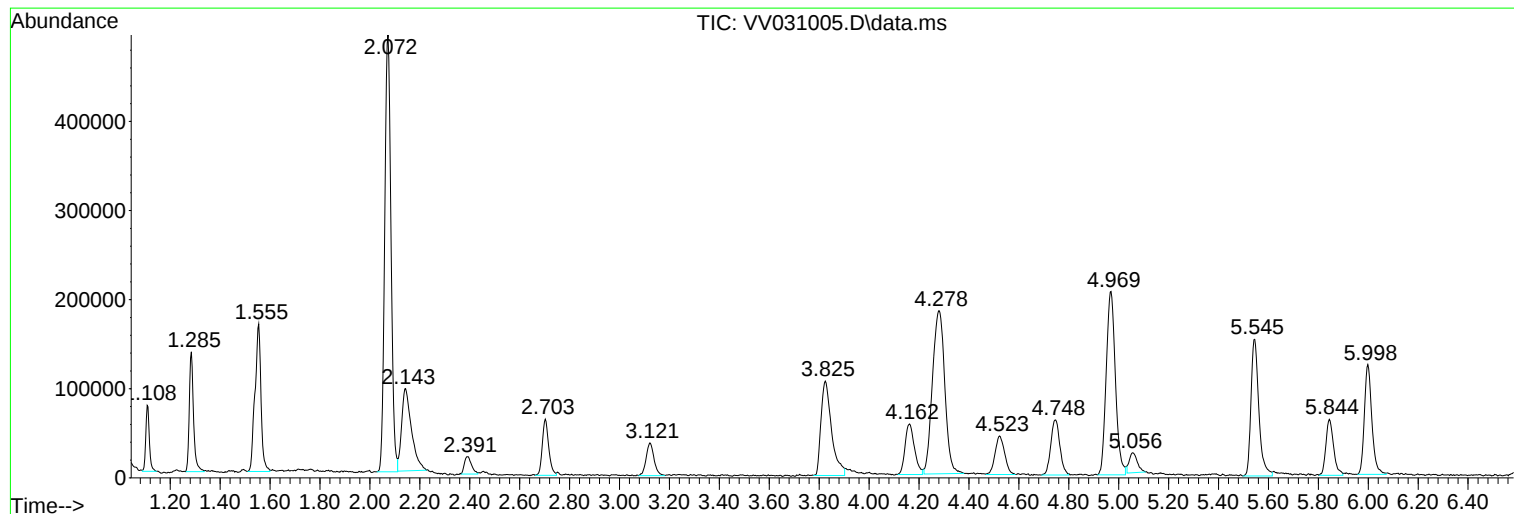

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031005.D
Acq On : 08 May 2023 13:16
Operator : SY/MD
Sample : 02614-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
X3G07










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3,5-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.590	3.29 ug/L	372053	1,4-Dichlorobenzene-d4	11.194

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
3			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
4			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
5			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	96

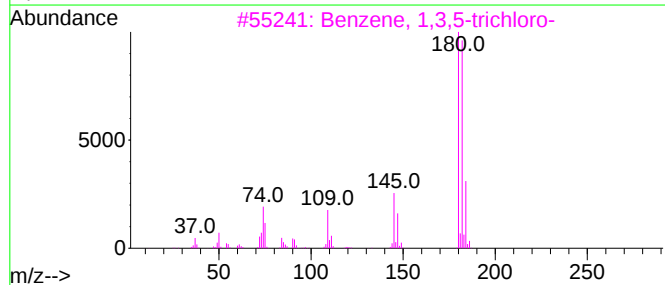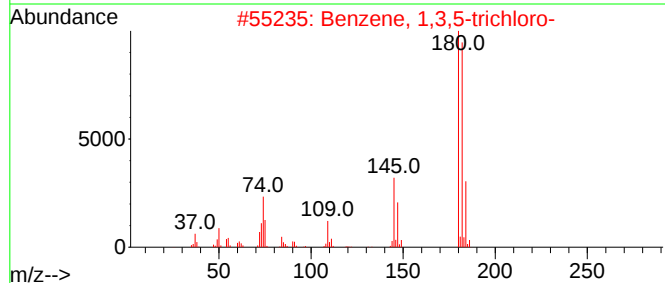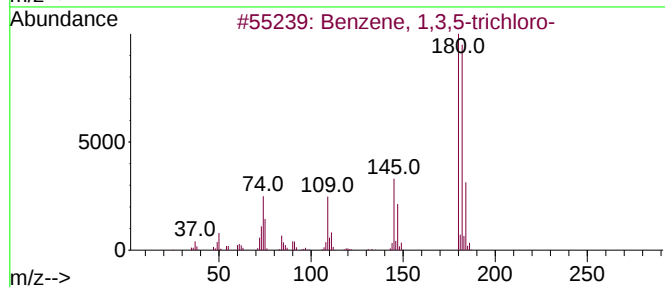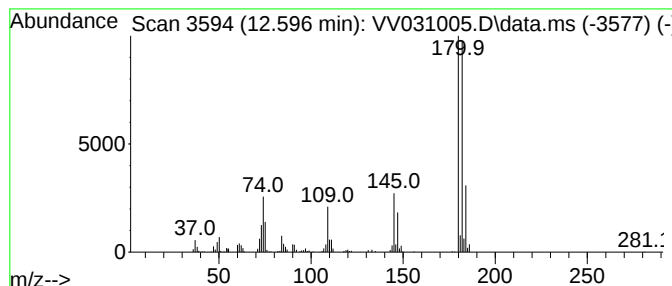

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031005.D
Acq On : 08 May 2023 13:16
Operator : SY/MD
Sample : 02614-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
X3G07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	12.590	3.3	ug/L	372053	3	11.194	565772	5.0