


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050823\
Data File : VV031001.D
Acq On : 08 May 2023 09:24
Operator : SY/MD
Sample : BFB259
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB259

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat May 06 01:44:36 2023

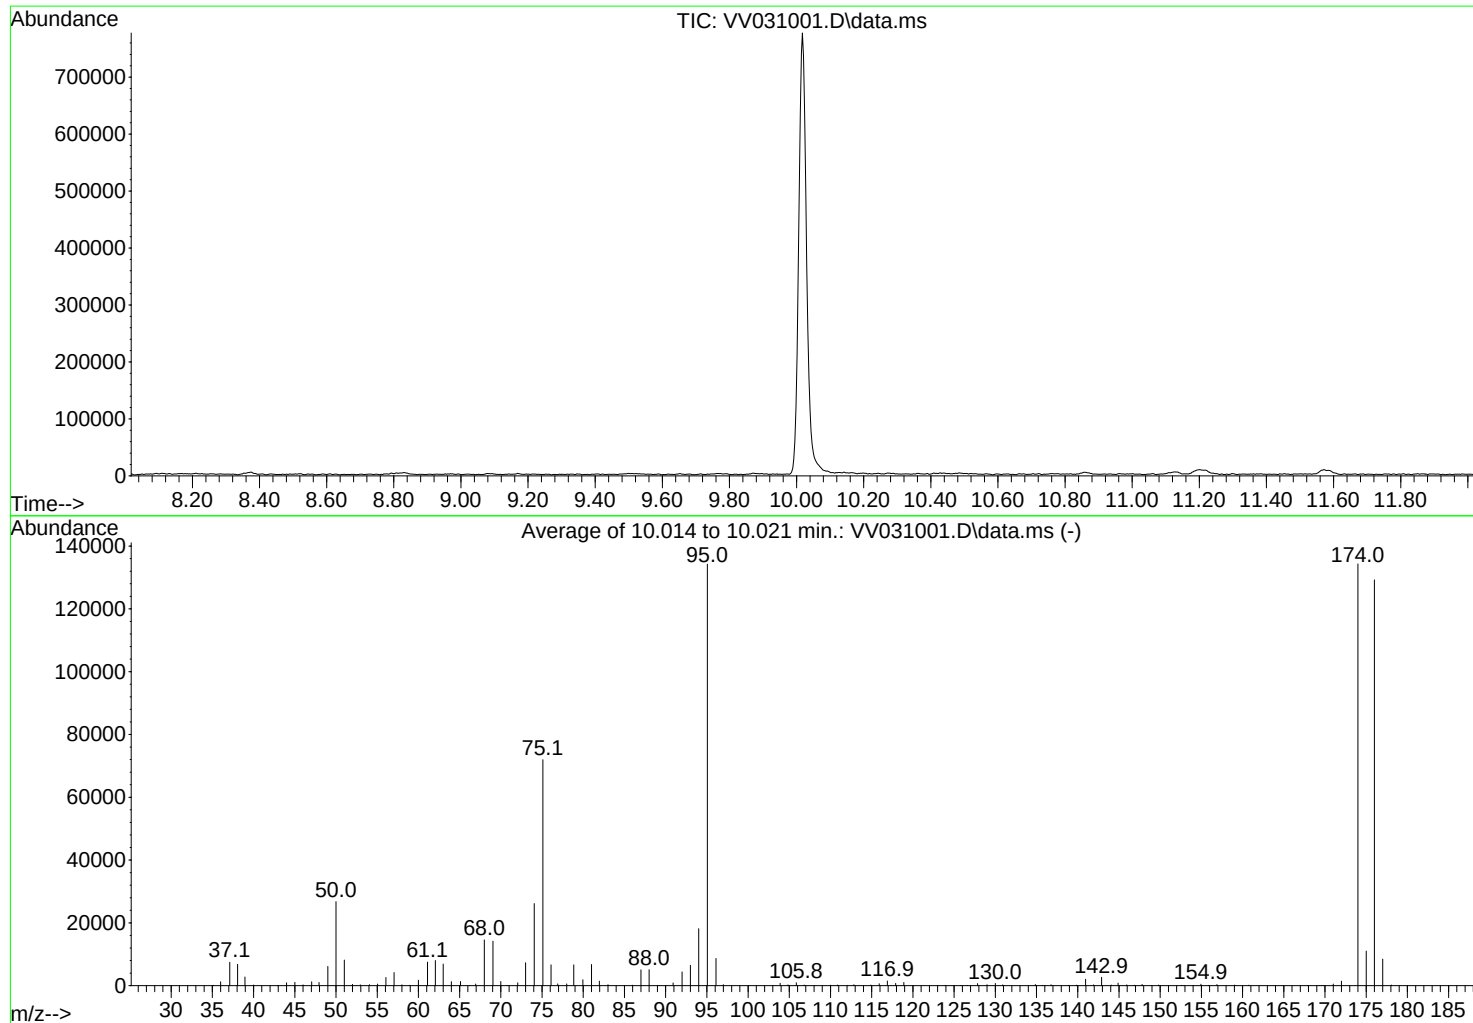

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	26753	PASS
75	95	30	80	53.6	71944	PASS
95	95	100	100	100.0	134208	PASS
96	95	5	9	6.4	8644	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	100.1	134336	PASS
175	174	5	9	8.2	10985	PASS
176	174	95	105	96.2	129253	PASS
177	176	5	10	6.5	8449	PASS

m/z	Abundance
35.50	108.0
36.00	145.0
37.20	100.0
38.40	134.0
38.80	174.0
40.00	236.0
40.80	214.0
41.70	104.0
42.90	153.0
44.00	290.0
45.10	138.0
46.40	127.0
47.80	107.0
50.00	116.0
51.00	105.0
52.00	128.0
54.80	107.0
55.60	116.0
58.00	105.0
61.70	101.0
66.30	131.0
72.40	105.0
76.90	103.0
78.80	101.0
85.90	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.20	137.0
36.00	1322.0
37.10	7697.0
38.10	6947.0
39.00	2894.0
40.00	403.0
41.00	171.0
43.00	143.0
44.00	1328.0
45.00	1269.0
46.00	310.0
47.00	1380.0
48.00	1163.0
49.00	6238.0
50.10	26856.0
51.00	8155.0
52.10	513.0
52.90	253.0
54.00	321.0
55.10	482.0
56.00	2529.0
57.10	4155.0
58.00	375.0
58.90	158.0
60.00	1725.0
61.10	7596.0
62.10	8045.0
63.00	6589.0
64.00	1197.0
65.10	1256.0
66.20	198.0
66.90	522.0
68.00	14352.0
69.00	14250.0
70.00	1263.0
70.80	133.0
72.10	881.0
73.00	7369.0
74.10	26144.0
75.10	71080.0
76.10	6696.0
76.90	707.0
78.00	513.0
78.90	6818.0
79.90	1904.0
81.00	6567.0
82.00	1383.0
83.00	327.0
86.00	331.0
87.00	5194.0
88.00	5066.0
89.20	121.0
90.90	882.0
92.00	4358.0
93.00	6478.0
94.00	17560.0
95.00	134592.0
96.10	8640.0
97.00	269.0
103.90	756.0
104.80	259.0
105.80	862.0
106.80	193.0
110.00	152.0
110.80	238.0
112.90	327.0
115.00	156.0
115.90	608.0
116.90	1605.0
117.90	708.0
118.90	1057.0
123.90	146.0
127.90	589.0
129.00	282.0
130.00	758.0
130.90	291.0
134.90	314.0
136.70	334.0
138.80	150.0
139.80	179.0
140.90	2058.0
141.90	247.0
142.90	2271.0
144.10	165.0
144.90	812.0
145.90	312.0
146.80	174.0
147.80	439.0
149.80	206.0
152.60	130.0
155.00	490.0
155.80	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

156.90	339.0
159.00	179.0
160.80	170.0
169.60	188.0
171.00	428.0
172.00	1317.0
174.00	131008.0
175.00	10921.0
176.00	125336.0
177.00	8633.0
178.00	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
35.10	149.0
36.00	1456.0
37.10	7742.0
38.00	6944.0
39.00	3049.0
40.10	451.0
40.90	213.0
42.90	152.0
44.00	1266.0
45.00	1251.0
46.00	240.0
47.00	1240.0
48.00	1180.0
49.00	6278.0
50.10	27624.0
51.00	8579.0
52.10	537.0
52.90	291.0
54.00	310.0
55.00	511.0
56.00	2620.0
57.00	4347.0
58.00	354.0
58.90	150.0
60.00	1785.0
61.10	7669.0
62.10	8429.0
63.00	7083.0
64.00	1389.0
65.10	1404.0
66.20	193.0
66.90	530.0
68.00	15056.0
69.10	14399.0
70.00	1362.0
72.10	929.0
73.00	7528.0
74.10	27184.0
75.10	74680.0
76.10	6924.0
77.00	679.0
78.00	570.0
78.90	6973.0
79.90	1935.0
81.00	6913.0
82.00	1531.0
83.00	312.0
86.00	331.0
87.00	5283.0
88.00	5303.0
89.20	107.0
90.90	874.0
92.00	4585.0
93.00	6706.0
94.00	18880.0
95.00	138560.0
96.10	8935.0
97.00	300.0
103.00	155.0
103.90	782.0
104.90	271.0
105.80	962.0
106.80	212.0
110.00	175.0
110.80	223.0
112.10	168.0
112.80	301.0
114.90	219.0
115.90	601.0
116.90	1581.0
117.90	736.0
118.90	1032.0
123.90	129.0
125.00	101.0
125.80	100.0
126.60	102.0
127.80	719.0
129.00	324.0
130.00	753.0
130.90	283.0
134.80	371.0
135.70	127.0
136.70	313.0
138.80	127.0
139.90	176.0
141.00	2139.0
141.90	277.0
142.90	2740.0
144.00	222.0
144.90	863.0
146.00	287.0
146.80	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

147.80	424.0
149.80	232.0
152.60	124.0
152.90	137.0
154.00	165.0
155.00	446.0
155.90	124.0
156.90	375.0
159.10	239.0
160.80	148.0
169.60	168.0
171.00	514.0
172.00	1508.0
174.00	139008.0
175.00	11304.0
176.00	133632.0
177.00	8685.0
178.00	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

m/z	Abundance
36.00	1418.0
37.10	7204.0
38.10	6481.0
39.00	2928.0
40.00	471.0
40.90	225.0
41.90	150.0
42.90	205.0
44.00	1103.0
45.00	1147.0
46.00	155.0
47.10	1071.0
48.00	1119.0
49.00	5878.0
50.00	26128.0
51.00	8060.0
52.00	523.0
53.00	297.0
54.10	253.0
55.00	510.0
56.10	2593.0
57.00	4096.0
58.00	293.0
60.00	1706.0
61.10	7209.0
62.00	7486.0
63.00	6896.0
64.00	1283.0
65.10	1344.0
66.20	169.0
67.00	495.0
68.00	14287.0
69.00	13853.0
70.00	1354.0
72.00	924.0
73.00	7010.0
74.00	25056.0
75.10	70072.0
76.10	6320.0
77.00	626.0
78.00	570.0
78.90	6426.0
80.00	1803.0
81.00	6761.0
81.90	1433.0
83.00	295.0
86.00	244.0
87.00	4707.0
88.00	4994.0
90.90	833.0
92.00	4262.0
93.00	6325.0
94.00	17928.0
95.10	129472.0
96.10	8356.0
97.00	301.0
103.00	160.0
103.90	711.0
104.90	296.0
105.90	938.0
106.80	169.0
108.10	121.0
110.00	149.0
110.90	181.0
112.10	200.0
112.90	236.0
114.80	247.0
115.90	628.0
116.90	1313.0
117.90	767.0
118.90	992.0
123.00	113.0
123.90	116.0
124.90	101.0
125.80	115.0
127.80	760.0
129.00	279.0
130.00	640.0
130.90	230.0
134.80	434.0
135.80	125.0
136.10	110.0
136.80	269.0
138.90	114.0
139.90	139.0
141.00	1925.0
141.90	313.0
142.90	2915.0
144.00	226.0
144.90	861.0
146.00	240.0
146.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259

147.80	398.0
148.90	114.0
149.80	211.0
152.90	151.0
154.00	205.0
154.90	388.0
155.90	110.0
156.90	360.0
159.10	265.0
160.70	117.0
167.90	113.0
169.30	104.0
169.80	124.0
171.00	537.0
172.00	1519.0
174.00	132992.0
175.00	10731.0
176.00	128792.0
177.00	8029.0
178.10	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB259