


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051120\
Data File : VV015988.D
Acq On : 11 May 2020 14:38
Operator : SY/MD
Sample : L2520-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41Y5

Manual Integrations
APPROVED

apatel
5/12/2020 11:07:52 AM

Quant Time: May 12 02:45:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 12 01:07:44 2020
Response via : Initial Calibration

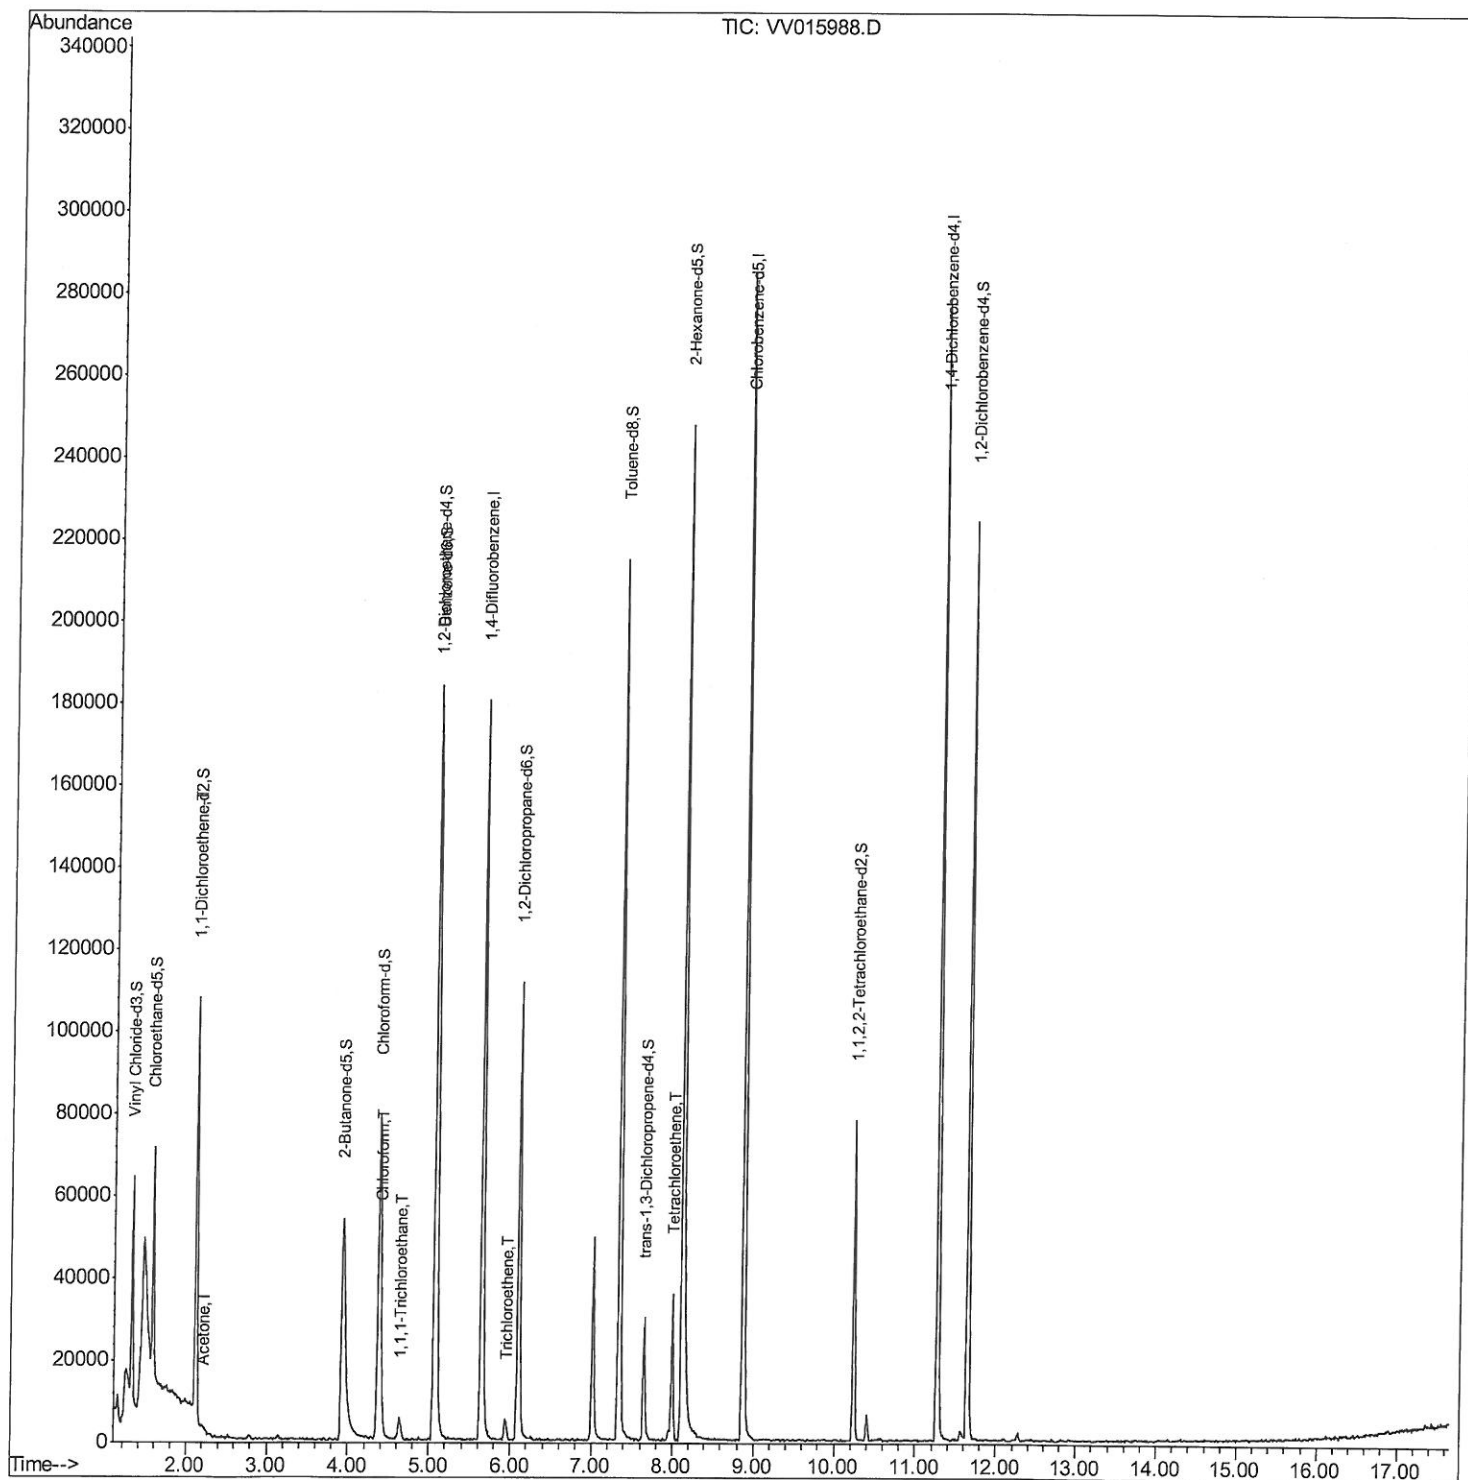

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051120\
 Data File : VV015988.D
 Acq On : 11 May 2020 14:38
 Operator : SY/MD
 Sample : L2520-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41Y5

Manual Integrations
 APPROVED

apatel
 5/12/2020 11:07:52 AM

Quant Time: Mav 12 02:41:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 12 01:07:44 2020
 Response via : Initial Calibration

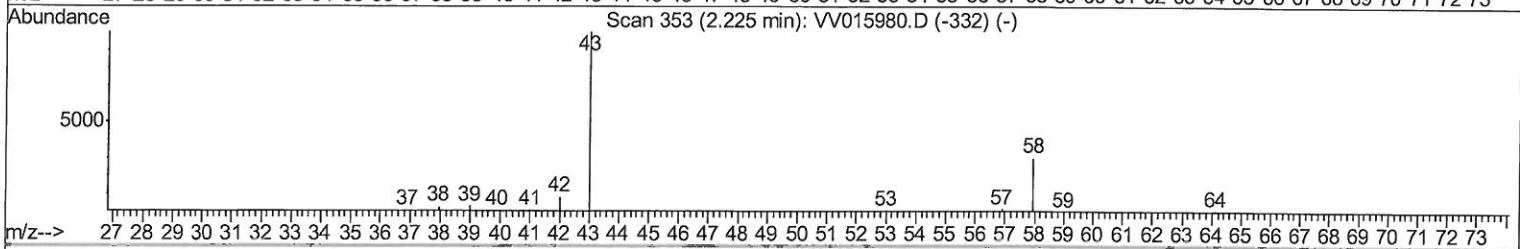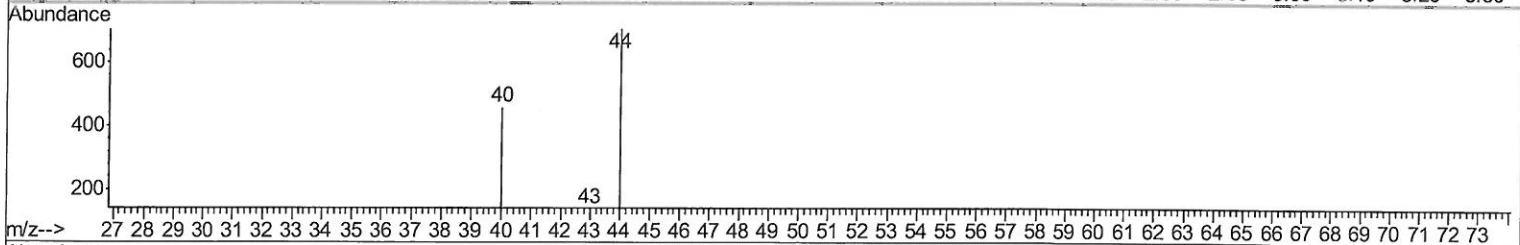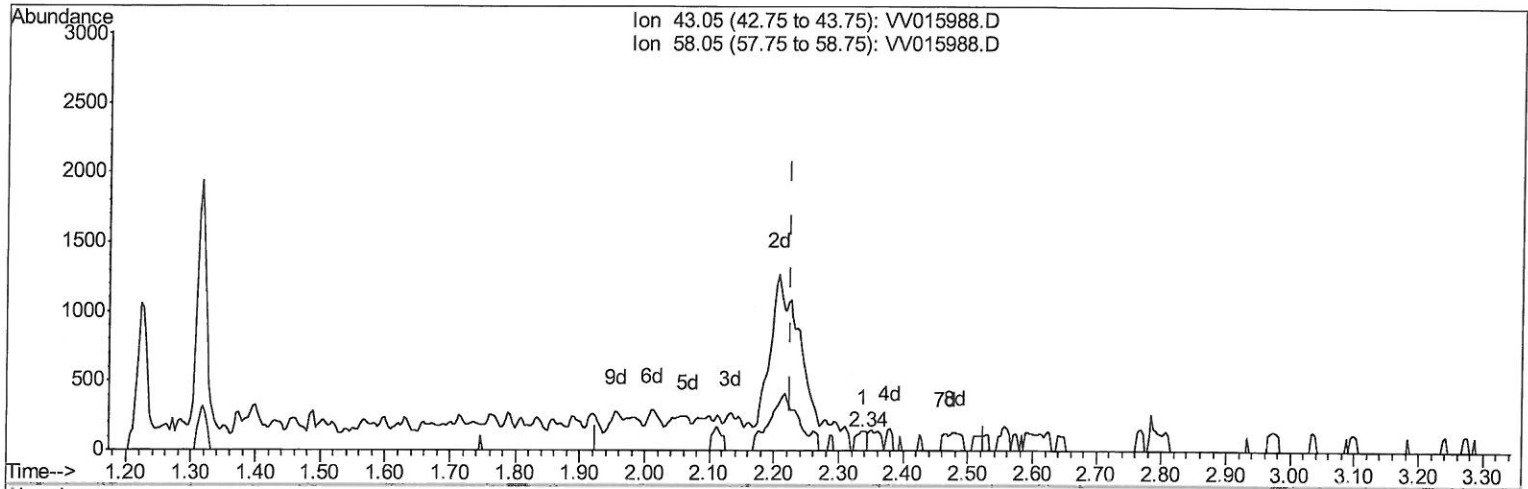

TIC: VV015988.D

(13) Acetone (T)

2.338min (+0.112) 0.12ug/L

response 172

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	25.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051120\
Data File : VV015988.D
Acq On : 11 May 2020 14:38
Operator : SY/MD
Sample : L2520-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41Y5

Manual Integrations
APPROVED

apatel
5/12/2020 11:07:52 AM

Quant Time: Mav 12 02:41:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 12 01:07:44 2020
Response via : Initial Calibration

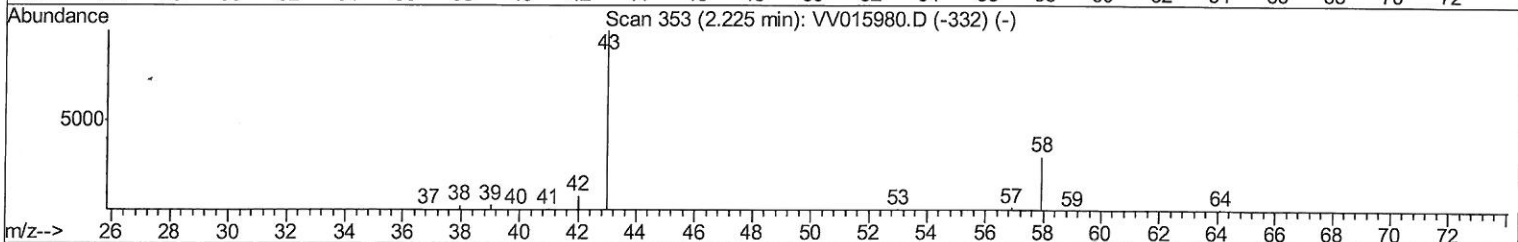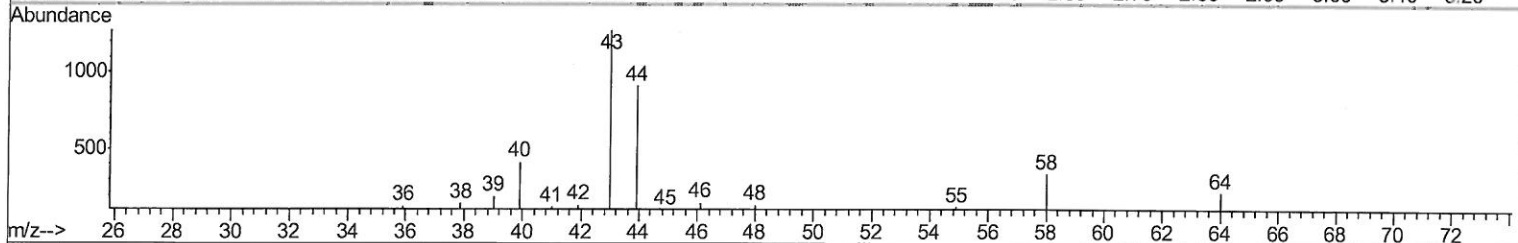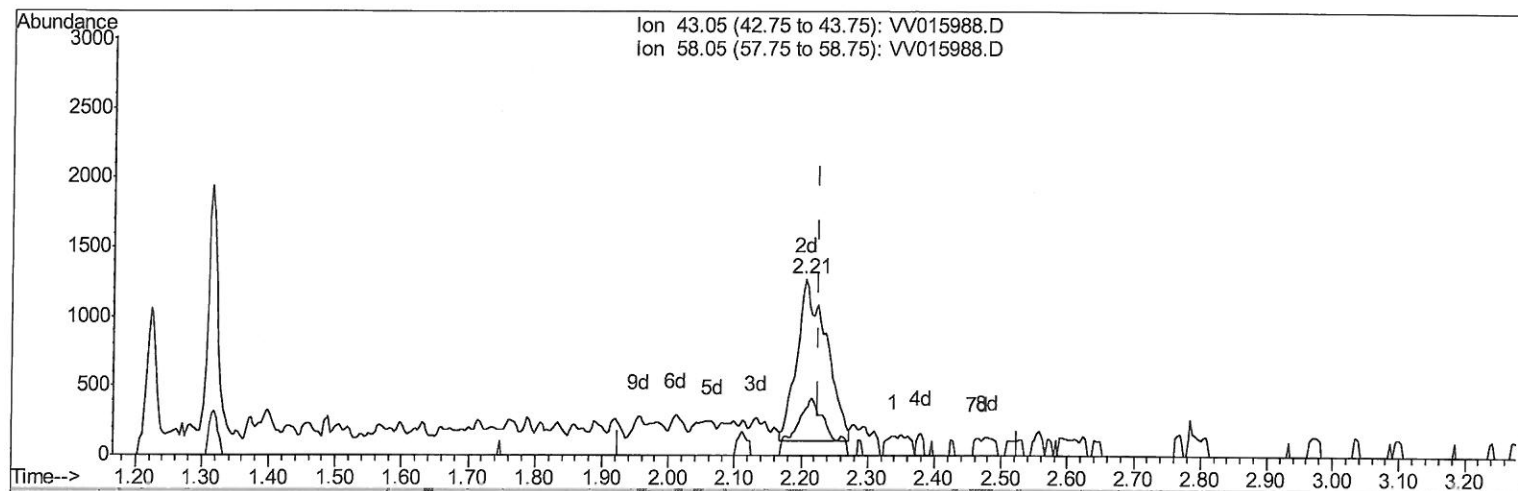

TIC: VV015988.D

(13) Acetone (T)

2.206min (-0.019) 2.44ug/L m

response 3606

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	1.19
0.00	0.00	0.00
0.00	0.00	0.00

MD
5/13/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051120\
 Data File : VV015988.D
 Acq On : 11 May 2020 14:38
 Operator : SY/MD
 Sample : L2520-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41Y5

Manual Integrations
 APPROVED

apatel
 5/12/2020 11:07:52 AM

Quant Time: May 12 02:45:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 12 01:07:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	144609	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	142834	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	65200	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	30016	3.83	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	76.60%		
7) Chloroethane-d5	1.58	69	31675	4.26	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	85.20%		
11) 1,1-Dichloroethene-d2	2.12	63	53733	3.19	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	63.80%		
20) 2-Butanone-d5	3.93	46	116742	52.17	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	104.34%		
24) Chloroform-d	4.38	84	77653	4.53	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	90.60%		
26) 1,2-Dichloroethane-d4	5.06	65	46698	4.75	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	95.00%		
32) Benzene-d6	5.08	84	152253	4.48	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.60%		
36) 1,2-Dichloropropane-d6	6.10	67	49951	4.82	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	96.40%		
41) Toluene-d8	7.34	98	137754	4.29	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	85.80%		
45) trans-1,3-Dichloropropene-	7.65	79	16999	4.18	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	83.60%		
48) 2-Hexanone-d5	8.12	63	82455	46.10	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	92.20%		
59) 1,1,2,2-Tetrachloroethane-	10.24	84	35281	4.84	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	96.80%		
65) 1,2-Dichlorobenzene-d4	11.65	152	53066	5.01	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	100.20%		
Target Compounds						
12) 1,1-Dichloroethene	2.13	96	6004	0.754	ug/L	1
13) Acetone	2.21	43	3606m	2.443	ug/L	
25) Chloroform	4.41	83	6509	0.349	ug/L	96
29) 1,1,1-Trichloroethane	4.64	97	4170	0.265	ug/L	99
34) Trichloroethene	5.95	95	1138	0.111	ug/L	94
49) Tetrachloroethene	8.00	164	7706	1.077	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2 m8
 5/13/20